



- (51) **International Patent Classification:**
A61B 5/00 (2006.01) *A61B 5/113* (2006.01)
A61B 5/08 (2006.01)
- (21) **International Application Number:**
PCT/US2017/046024
- (22) **International Filing Date:**
09 August 2017 (09.08.2017)
- (25) **Filing Language:** English
- (26) **Publication Language:** English
- (30) **Priority Data:**
62/382,104 31 August 2016 (31.08.2016) US
62/395,218 15 September 2016 (15.09.2016) US
- (71) **Applicant: THE BOARD OF REGENTS OF THE UNIVERSITY OF TEXAS SYSTEM** [US/US]; 201 West Seventh Street, Austin, TX 78701 (US).
- (72) **Inventor: CHIAO, Jung-Chih**; c/o The Board of Regents of the University of Texas System, 201 West Seventh Street, Austin, TX 78701 (US).
- (74) **Agent: ROBINSON, Eagle, H.**; Norton Rose Fulbright US LLP, 98 San Jacinto Blvd., Suite 1100, Austin, TX 78701 (US).
- (81) **Designated States** (*unless otherwise indicated, for every kind of national protection available*): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DJ, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IR, IS, JO, JP, KE, KG, KH, KN, KP, KR, KW, KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(54) **Title:** NON-INVASIVE SAMPLE-INTERROGATION DEVICE

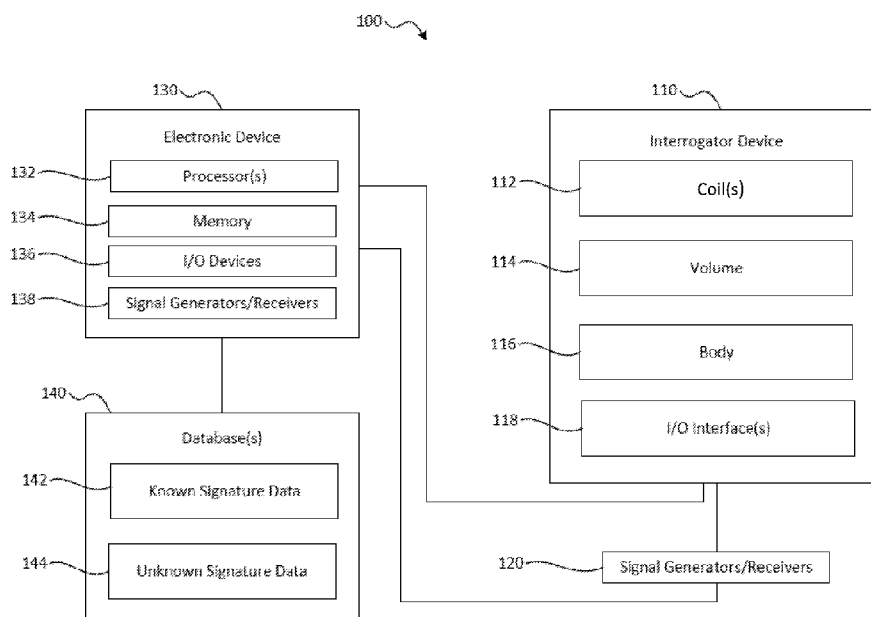


FIG. 1

(57) **Abstract:** Embodiments of the present disclosure provide an interrogation device that is operable to apply one or more source signals to one or more coils surrounding a volume, where a material is disposed within the volume. Each of the one or more source signals may excite one of the one or more coils, and the behavior of each the one or more coils responsive to the exciting may be monitored. One or more parameters may be determined based on the behavior of each the one or more coils, and the one or more parameters may be utilized to generate a signature for the material within the volume. The signature may be compared to one or more signatures of known materials to identify the material within the volume.



(84) Designated States (*unless otherwise indicated, for every kind of regional protection available*): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, ST, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, KM, ML, MR, NE, SN, TD, TG).

Published:

— *with international search report (Art. 21(3))*

DESCRIPTION

NON-INVASIVE SAMPLE-INTERROGATION DEVICE

CROSS-REFERENCE TO RELATED APPLICATIONS

[0001] This application claims priority to United States Provisional Patent Application
5 No. 62/395,218 filed September 15, 2016, and to United States Provisional Patent
Application No. 62/382,104 filed August 31, 2016, the contents of all of which applications
are incorporated by reference.

FIELD OF INVENTION

[0002] The present disclosure is generally directed to non-intrusive materials analysis
10 techniques, and more particularly to liquid component analysis and characterization using
scattering parameters and/or Smith charts.

BACKGROUND

[0003] Typically, testing of liquids and other materials to determine the contents thereof
is performed using chemically-reactive processes. Such processes introduce new substances
15 into the sample being tested, which may cause a tested sample to become unfit for additional
testing. In such scenarios, a different sample is needed for each different type of test to be
performed, and is typically performed manually.

SUMMARY

[0004] The present disclosure provides systems, methods, and computer-readable storage
20 media operable to analyze an unknown material to identify one or more characteristics of the
material. In some embodiments, a material (e.g., an unknown material) may be placed in a
volume (e.g., an interior channel of a body) that is surrounded by one or more coils. While
the material is within the volume, the one or more coils may be excited, and the behavior of
the one or more coils while excited may be monitored to observe one or more parameters
25 associated with the behavior of the one or more coils. For example, the one or more
parameters observed during the monitoring may be scattering parameters or S-parameters.
The one or more parameters may be used to generate one or more signatures for the unknown
material, which may then be compared to signatures of known materials to identify the

presence of one or more of the known materials in the unknown material. For example, some embodiments may detect the presence of a first liquid, such as vodka, and may be operable to distinguish when the first liquid is present in its pure form and when the first liquid has been diluted by a second liquid, such as water. In some embodiments, the signature may be an
5 Smith Chart generated based on the one or more parameters that were observed during excitement of the one or more coils.

[0005] In some embodiments, a plurality of signatures, such as a plurality of Smith Charts, may be generated. In embodiments, some of the plurality of signatures may be generated by exciting the coils at different frequencies, which may alter the behavior of the
10 coils for a particular observation of the one or more parameters (e.g., the one or more parameters may exhibit different values at different frequencies). This may provide a plurality of signatures that may be used to identify the liquid. For example, a plurality of Smith Charts representing the behavior of the one or more coils when excited at different frequencies may be generated. Increasing the number of signatures for a liquid may increase
15 the reliability of a system configured to identify a liquid according to embodiments.

[0006] The term “coupled” is defined as connected, although not necessarily directly, and not necessarily mechanically. The terms “a” and “an” are defined as one or more unless this disclosure explicitly requires otherwise. The term “substantially” is defined as largely but not necessarily wholly what is specified (and includes what is specified; e.g., substantially
20 90 degrees includes 90 degrees and substantially parallel includes parallel), as understood by a person of ordinary skill in the art. In any disclosed embodiment, the terms “substantially” and “approximately” may be substituted with “within [a percentage] of” what is specified, where the percentage includes 0.1, 1, 5, and 10%.

[0007] Further, a device or system that is configured in a certain way is configured in at
25 least that way, but it can also be configured in other ways than those specifically described.

[0008] The terms “comprise” (and any form of comprise, such as “comprises” and “comprising”), “have” (and any form of have, such as “has” and “having”), “include” (and any form of include, such as “includes” and “including”), and “contain” (and any form of contain, such as “contains” and “containing”) are open-ended linking verbs. As a result, an
30 apparatus that “comprises,” “has,” “includes,” or “contains” one or more elements possesses those one or more elements, but is not limited to possessing only those elements. Likewise, a method that “comprises,” “has,” “includes,” or “contains” one or more steps possesses those one or more steps, but is not limited to possessing only those one or more steps.

[0009] Any embodiment of any of the apparatuses, systems, and methods can consist of or consist essentially of – rather than comprise/include/contain/have – any of the described steps, elements, and/or features. Thus, in any of the claims, the term “consisting of” or “consisting essentially of” can be substituted for any of the open-ended linking verbs recited
5 above, in order to change the scope of a given claim from what it would otherwise be using the open-ended linking verb.

[0010] The feature or features of one embodiment may be applied to other embodiments, even though not described or illustrated, unless expressly prohibited by this disclosure or the nature of the embodiments.

10 [0011] Some details associated with the embodiments described above and others are described below.

BRIEF DESCRIPTION OF THE DRAWINGS

[0012] The following drawings illustrate by way of example and not limitation. For the sake of brevity and clarity, every feature of a given structure is not always labeled in every
15 figure in which that structure appears. Identical reference numbers do not necessarily indicate an identical structure. Rather, the same reference number may be used to indicate a similar feature or a feature with similar functionality, as may non-identical reference numbers.

[0013] FIG. 1 is a block diagram of a system for identifying an unknown material according to embodiments of the present disclosure;

20 [0014] FIG. 2 is an illustrative embodiment of an interrogator device according to embodiments of the present disclosure;

[0015] FIG. 3A is a diagrams illustrating a side view of a body and coil arrangement according to an embodiment of the present disclosure;

[0016] FIG. 3B is a diagrams illustrating a top view of a body and coil arrangement
25 according to an embodiment of the present disclosure;

[0017] FIG. 3C is a diagrams illustrating a schematic view of a body and coil arrangement according to an embodiment of the present disclosure;

[0018] FIG. 4 is a flow diagram of an exemplary method for identifying an unknown material according to embodiments of the present disclosure;

30 [0019] FIG. 5 is a graph illustrating various characteristics of different liquids that have been interrogated according to embodiments of the present disclosure;

[0020] FIG. 6 is a chart illustrating characteristics observed during interrogation of liquids containing alcohol at different concentrations according to embodiments of the present disclosure;

5 [0021] FIG. 7 is a diagram illustrating a plot of resonant frequencies observed during interrogation of liquids containing alcohol at different concentrations;

[0022] FIG. 8 is a diagram illustrating a plot of the minimum |S₁₁| peaks observed during interrogation of liquids containing alcohol at different concentrations;

[0023] FIG. 9 is a diagram illustrating Smith charts generated based on observations during interrogation of liquids containing alcohol at different concentrations;

10 [0024] FIG. 10 is a chart illustrating characteristics observed during interrogation of liquids containing milk at different concentrations according to embodiments of the present disclosure;

[0025] FIG. 11 is a diagram illustrating a plot of resonant frequencies observed during interrogation of liquids containing milk at different concentrations;

15 [0026] FIG. 12 is a diagram illustrating a plot of the minimum |S₁₁| peaks observed during interrogation of liquids containing milk at different concentrations;

[0027] FIG. 13 is a diagram illustrating Smith charts generated based on observations during interrogation of liquids containing milk at different concentrations;

20 [0028] FIG. 14 is a chart illustrating characteristics observed during interrogation of liquids containing different milk/alcohol mixes according to embodiments of the present disclosure;

[0029] FIG. 15 is a diagram illustrating a plot of resonant frequencies observed during interrogation of liquids containing different milk/alcohol mixes according to embodiments;

25 [0030] FIG. 16 is a diagram illustrating a plot of the minimum |S₁₁| peaks observed during interrogation of liquids containing different milk/alcohol mixes;

[0031] FIG. 17 is a diagram illustrating Smith charts generated based on observations during interrogation of liquids containing different milk/alcohol mixes;

[0032] FIG. 18A is a diagram illustrating aspects of an embodiment of an interrogator comprising a plurality of coils according to the present disclosure;

30 [0033] FIG. 18B is a diagram illustrating aspects of an embodiment of an interrogator comprising a plurality of coils according to the present disclosure;

[0034] FIG. 19 is a diagram illustrating aspects of an embodiment for performing classification of a liquid using a signature generated according to embodiments;

[0035] FIG. 20 is a diagram illustrating additional aspects of an embodiment for performing classification of a liquid using a signature generated according to embodiments;

[0036] FIG. 21 is a diagram illustrating an embodiment of an interrogator device having a body surrounded by 2 coils;

5 **[0037]** FIG. 22 is a diagram illustrating an embodiment of an additional technique for identifying an unknown liquid using Smith Charts and the related resonant frequencies according to the present disclosure.

[0038] FIG. 23 is a diagram illustrating an embodiment of an additional technique for identifying an unknown liquid using a different arrangements of the coils according to the
10 present disclosure

[0039] FIG. 24 is a diagram illustrating an embodiment of an additional technique for identifying an unknown liquid using a plurality of coils according to the present disclosure

[0040] FIG. 25 is a chart of the observed parameters measured during various arrangements.

15 **[0041]** FIG. 26 is a chart showing the use of parameters of several liquids to cross check the observed parameters in order to generate more signatures. FIG. 27 is a flow diagram of exemplary method for identifying an unknown material in accordance with embodiments of the present disclosure;

[0042] FIG 28 is a diagram that illustrates additional aspects of frequency ranges that
20 may be used to identify a material according to embodiments;

[0043] FIG. 29 is a diagram illustrating aspects of a graphical user interface (GUI) for configuring a system for interrogation of a sample of an unknown material;

[0044] FIG. 30 is another diagram illustrating aspects of a graphical user interface (GUI) for configuring a system for interrogation of a sample of an unknown material;

25 **[0045]** FIG. 31 is another diagram illustrating aspects of a graphical user interface (GUI) for configuring a system for interrogation of a sample of an unknown material;

[0046] FIG. 32 is a diagram illustrating aspects of functional relationships and software modules that may be implemented in an interrogation system configured according to embodiments;

30 **[0047]** FIG. 33 is a diagram illustrating aspects of functional relationships and software modules that may be implemented in an interrogation system configured according to embodiments; and

FIG. 34 is a diagram illustrating aspects of functional relationships and software modules that may be implemented in an interrogation system configured according to embodiments.

DETAILED DESCRIPTION OF ILLUSTRATIVE EMBODIMENTS

[0048] Referring now to the drawings, and more particularly to FIG. 1, an embodiment of a system operable to perform interrogation of a material (e.g., an unknown material) and to identify one or more characteristics of the material is shown as a system 100. For example, various components of system 100 may cooperate to allow an unknown material to be identified. In some embodiments, the material comprises water, alcohol, coffee, a soft drink, milk, oil, blood, or a combination thereof. It is noted however, that the exemplary materials described in the various embodiments of the present disclosure are provided for purposes of illustration, rather than by way of limitation. Thus, the present disclosure is not to be limited to the particular materials described herein, as the concepts of the various embodiments of the present disclosure can be readily applied to identification of other materials.

[0049] Where the unknown material is a liquid, the system 100 may interrogate a sample of the unknown liquid, and, as described in more detail below, based on the analysis, may identify one or more characteristics of the liquid, such as one or more types of liquid contained within the sample. For example, an exemplary system 100 configured according to embodiments of the present disclosure has been demonstrated to be operable to detect and/or identify the presence of various concentrations of alcohol in de-ionized water, as described in more detail below with reference to FIGs. 6-9. In some embodiments, other types of analysis may be performed by the system 100, such as to determine the moisture content of soil or when a liquid changes from a first state (e.g., a liquid) to a second state (e.g., a solid). Additional types and description of the analysis that may be performed using the system 100 are described below.

[0050] As shown in FIG. 1, interrogator device 110 comprises one or more coils 112, a volume 114, a body 116, and one or more input/output (I/O) interfaces 118. In alternate embodiments one or more single strip antenna(e) may be used in combination or as a replacement for the coils 112. Body 116 may define an interior channel, and volume 114 may be the space within the interior channel. A material that is to be tested/interrogated by system 100 may be placed directly within volume 114 (e.g., in the interior channel). In some embodiments, the material may be placed inside a container, such as a bottle, and the container placed in the volume 114. Interrogating a sample that has been placed in a container may allow the sample to be analyzed without corrupting or altering the sample, such by contamination of the sample with residue within the interior channel. This may result in analysis of samples with a higher degree of integrity and reduce the likelihood that

the contents of the sample are incorrectly identified. This may also enable system 100 to be utilized for testing samples that need to remain sealed, as described in more detail below. In some embodiments, the volume 114 may be sized and dimensioned to accommodate a variety of container sizes. In an additional or alternative embodiment, the volume 114 may be sized and dimensioned to accommodate a single container size, such as a test tube or another type of container specifically sized and dimensioned to be received in the interior channel of body 116. Additionally, it is noted that utilizing samples placed in containers may reduce the upkeep and maintenance of the system 100. For example, if the material is placed directly within the volume 114, the interior channel of the body 116 may need to be cleaned prior to interrogating/analyzing an additional sample of material, whereas when the material is placed in a container, the interior channel of the body 116 may not need to be cleaned prior to interrogating/analyzing an additional sample of material. This may increase the speed at which different samples may be analyzed by system 100, which may provide performance enhancements in some applications of system 100, as described in more detail below.

[0051] In some embodiments, each of coil(s) 112 may be coupled to body 116. For example, each of coil(s) 112 may be wrapped around an exterior surface of body 116. In some embodiments, an insulating material or cover may be placed over or around the outer surface of body 116 and coil(s) 112. The insulating material or cover may help maintain coil(s) 112 in a desired alignment and prevent damage to the coil(s). In some embodiments, the coil(s) 112 may comprise two or more coils. In some embodiments, at least one of coil(s) 112 comprises two or more turns (e.g., four or more turns). In some embodiments, a maximum transverse dimension of volume 114 may be about or substantially 4 centimeters (cm) or larger. In some embodiments, body 116 comprises a pipe through which the material flows. For example, in an industrial liquid treatment or processing facility, such as a wastewater treatment facility or a chemical processing or manufacturing facility, body 115 may be a pipe through which a liquid or liquids flow, and coil(s) 112 may be wrapped around the pipe to perform analysis of the liquid flowing through the pipe.

[0052] As shown in FIG. 1, one or more I/O interfaces 118 may communicatively couple the interrogator device to device 130 and/or the one or more signal generators/receivers 120.

More particularly, in some embodiments, I/O interface(s) 118 may couple each of coil(s) 112 to a respective one of the signal generators/receivers 138 of electronic device 130, or, in an additional or alternative embodiment, I/O interface(s) 118 may couple each of the one or more coils 112 to a respective one of the one or more signal generators/receivers 120. The one or more signal generators/receivers may be configured to excite each of coil(s) 112 with

a respective source signal, as described in more detail below. The exciting of coil(s) 112 may induce a behavior at each of the one or more coils, and the behavior of each of coil(s) 112 in response to the excitement may be monitored by the respective ones of the one or more signal generators/receivers. One or more parameters representative of the behavior of each of
5 coil(s) 112 may be monitored during the exciting of the coils. For example, exciting the coil(s) 112 with the respective source signal(s) may induce electromagnetic fields for each of the coil(s), and one or more parameters associated with coil(s) 112 and their respective electromagnetic field(s) may be observed, as described in more detail below.

[0053] In some embodiments, a matching circuit 122 may be coupled in series with the
10 coil(s). The matching circuit 122 may be used to match the impedance between two points of the interrogator device 100, such that power transfer is optimized to the coil(s) 112. Optimizing power transfer to the coils(s) 112 may increase the sensitivity of the signatures by generating more precise parameters. For example, a Pi matching circuit may be used to generate higher quality factors in resonance when identifying de-ionized water. The
15 matching circuit 122 may enhance sensitivity to other parameters used by the interrogator 100, as described in more detail below.

[0054] Electronic devices 130 may include a processor(s) 132, a memory 134, I/O
20 devices 136, and the one or more signal generators/receivers 138. In some embodiments, memory 134 may store instructions that, when executed by the processor(s) 132, cause processor(s) 132 to perform operations to analyze a material, for example, as described in more detail below. In some embodiments, the instructions comprise a software program that may be executed by processor(s) 132 to control operations of system 100 during interrogation and/or analysis of an unknown material in accordance with embodiments of the present disclosure, as described in more detail below. For example, the software program may
25 provide one or more graphical user interfaces (GUIs) that allow a user to configure one or more aspects of the interrogation and/or analysis, such as to configure one or more frequencies utilized to excite coil(s) 112 during interrogation and/or analysis of a sample of unknown material. Additionally, the one or more GUIs may include GUIs that enable the user to view one or more aspects of the analysis, such as to view information representative
30 of one or more parameters observed during the analysis, as described in more detail below. Thus, the software program may provide a suite of tools and functionality that enable analysis of a material in accordance with embodiments of the present disclosure.

[0055] In some embodiments, signal generators/receivers 138 may be configured to excite coil(s) 112 and to generate information representative of one or more parameters of

coil(s) 112 observed during the excitement of the coil(s) 112. In other embodiments the coil(s) may be used in addition to or replaced with antenna(e). In an additional or alternative embodiment, electronic device 130 may not include signal generators/receivers 138, and instead, may be communicatively coupled to one or more external signal generators/receivers 120 that is/are configured to excite coil(s) 112 and to provide to electronic device 130 information representative of one or more parameters of coil(s) 112 during the excitement. In some embodiments, signal generator(s)/receiver(s) 138 and/or signal generator(s)/receiver(s) 120 may comprise a vector network analyzer (VNA) configured to excite coil(s) 112 and provide information representative of observed parameters to electronic device 130. In some embodiments, irrespective of whether the signal generator(s)/receiver(s) are integral with or external to the electronic device, they may operate under control of electronic device 130. For example, the software program stored as instructions at memory 134 may provide one or more GUIs and tools to configure the analysis and interrogation of the material within interrogator device 110.

[0056] During the interrogation/monitoring of a material within interrogator device 110, one or more parameters may be observed for each of coil(s) 112 (e.g., based on the electromagnetic fields induced by the exciting of each of coil(s) 112). For example, in some embodiments, the one or more parameters observed during the monitoring may include: a self-resonance frequency, a reflection coefficient, a transmission coefficient, or a combination thereof. In some embodiments, the resonant frequencies may be indicated by the reflection and transmission coefficients. In some embodiments, the one or more signal generators/receivers may generate a data set that represents the one or more parameters observed during the monitoring as scattering parameters (S-parameters), as described in more detail below. The data set may be stored at a database, such as database 140, as unknown signature data 144, and may include values for each of the one or more parameters observed during the monitoring. For example, where the monitoring is performed with respect to scattering parameters, the data set may include a plurality of scattering parameters values observed over a range of frequencies, thus, providing a plurality of data points in a frequency range of interest (e.g., a frequency range at which the coils are excited during a particular analysis of a material or a particular portion of the analysis). It is noted that one or more of the observed parameters may vary depending on the configuration of each of coil(s) 112 (e.g., the number of wraps, dielectric materials proximate to each of the one or more coils 112, etc.) and the frequency of the source signal. In embodiments where the material is placed within volume 114 while inside a container, the container may be required to be a

container specially purposed for use with system 100 (e.g., because interrogation of the same liquid in different containers comprised of different materials may cause coil(s) 112 to exhibit different parameters). Processor 132 of electronic device 130 may analyze the data set to determine a signature associated with a material within volume 114. For example, in some

5 embodiments, the signature may be determined based on the one or more parameters observed during the monitoring. After determining the signature for the material undergoing interrogation, the processor 132 may retrieve one or more candidate signatures (e.g., from a data set of candidate signatures 142) from the data base 140, and compare the signature for the material undergoing interrogation to the one or more candidate signatures to identify one

10 or more characteristics of the material. In some embodiments, the data set of candidate signatures may comprise signatures generated by observing the behavior of coil(s) 112 during interrogation of known materials. Thus, comparing the candidate signatures of the data set of candidate signatures 142 may enable a signature for an unknown material to be matched with a signature of a known material in order to identify the material. In some embodiments, the

15 data set of candidate signatures may comprise a plurality of signatures for each known material. For example, multiple candidate signatures for a known material may be generated, where at least two of the candidate signatures are generated by interrogating a sample of the known material at different frequencies. The behavior of coil(s) 112 may vary depending on the frequency, and generating more candidate signatures at different frequencies may increase

20 the reliability of material identifications performed by system 100. Additionally, in some embodiments, multiple signatures for a known material may be generated at a single frequency, which may provide more reliable analysis under conditions where other variables may affect the analysis, such as changed in the temperature of liquid and/or the ambient environment where the testing is performed. In some embodiments, the one or more

25 characteristics may include an alcohol content of the material, a moisture content of the material (e.g., a moisture content of a sample of soil), a solids content of the material (e.g., a liquid material is transitioning to a solid, when the transition is complete, and the like), a plasma content of the material (e.g., a plasma content of a sample of blood), a temperature of the material, another characteristic, or a combination thereof.

30 **[0057]** In an embodiment, statistical analysis techniques may be utilized to perform the comparison of the unknown signature data 144 to the one or more candidate signatures 142. Such techniques may be utilized to determine whether the unknown signature data 144 matches a particular one of the one or more candidate signatures 142 to within a threshold tolerance or to within a threshold confidence interval. In an embodiment, the threshold

tolerance and/or threshold confidence interval may be configured to provide a desired degree of certainty with respect to identifying the material. For example, testing of samples of different liquid materials using a device configured according to the embodiment illustrated in FIG. 1 has demonstrated that the system of FIG. 1 can identify a material as being pure
5 (e.g., contains only one liquid) or contaminated (e.g., contains a primary liquid or material, such as milk, and one or more additional and different liquids and/or materials, such as alcohol, that have been mixed within primary liquid or material) with almost 100% accuracy. In an embodiment, the threshold tolerance and/or confidence interval may be configurable depending on a particular application of, and accuracy requirements for, the interrogation
10 system.

[0058] In some embodiments, the one or more candidate signatures may correspond to signatures representative of at least one known material that were determined based one or more parameters observed while the at least one known material was disposed within volume 114 of interrogator device 110. In some embodiments, the one or more candidate signatures
15 may be selected based at least in part on the frequency or frequencies used to excite coil(s) 112. For example, when coil(s) 112 is/are excited using a first set of frequencies, candidate signatures that were generated for known materials based on exciting the one or more coils at the first set of frequencies may be selected for comparison to the signature of the unknown material. In some embodiments, the frequency or frequencies at which the one or more coils
20 are excited may be varied during the monitoring. For example, data representative of the behavior of the induced electromagnetic fields may be observed at a first set of one or more frequencies, and then the one or more frequencies may be modified and additional data representative of the behavior of the induced electromagnetic fields may be observed. Obtaining data at multiple frequencies may enable a more accurate identification of the
25 material undergoing interrogation, such as to rule out known signatures that do not exhibit similar behaviors at one or more of the frequencies used to interrogate an unknown material and/or to identify known signatures that exhibit similar behaviors at one or more of the frequencies used to interrogate an unknown material. This may provide a coarse level of filtering that reduces the pool of known or candidate signatures that may correspond to the
30 signature of the material undergoing interrogation. In some embodiments, comparing, at each of the set of frequencies, the determined parameter (or behavior) with the corresponding known parameter (e.g., known signature) comprises comparing a Smith chart of the determined parameter with a Smith chart of the corresponding known parameter, as described in more detail below. Additional aspects of embodiments for interrogating a material and

techniques for identifying the material (and/or characteristics of the material) based on parameters observed during the interrogating are described below.

[0059] From the foregoing it is shown that embodiments of system 100 provide techniques for non-invasively interrogating and identifying a material (e.g., an unknown material) and/or characteristics of the interrogated material. That is, embodiments of the present disclosure enable interrogation and analysis of a sample of a material without corrupting or altering the sample, such by contamination of the sample with residue within the interior channel of body 116. This can result in analysis of samples with a higher degree of integrity and reduce the likelihood that the contents of the sample are incorrectly identified. Further, as described in more detail below, embodiments of system 100 have been demonstrated to identify materials with a high degree of reliability. Thus, the present embodiments may, for example, provide an improved technique for identifying unknown materials.

[0060] FIG. 2 depicts an embodiment of the present interrogator devices and is shown as an interrogator device 210 (and may, for example, correspond to or be used in place of interrogator device 110 in system 100 of FIG. 1). In the embodiment shown, interrogator device 210 may comprise a housing 220, a coil 212, a body 222 defining an interior channel within a volume 214, and one or more I/O interfaces 216. In some embodiments, a stabilizer material 224 may be utilized to stabilize the orientation of body 222 within housing 220. Coil 212 may be wrapped around the body 222, and may be coupled to I/O interface(s) 216. During analysis, a sample of a material may be disposed within volume 214 (e.g., within the interior channel defined by body 222), coil 212 may be excited, and one or more parameters associated with an electromagnetic field associated with coil 212 may be observed. The unknown material may then be identified based on the observed parameters of the induced electromagnetic field of coil 212, as described in more detail below.

[0061] FIGs. 3A-3C illustrate respectively side, top, and schematic views of a body and coil arrangement according to one of the present embodiments. As shown in FIGs. 3A and 3B, the body (e.g., body 116 of FIG. 1) may have a height of approximately 9.7 centimeters (cm) and a width of approximately 4.2 cm. As shown in FIG. 3A, the coil (e.g., a coil 112 of FIG. 1) may comprise a plurality of wraps that surround the body and are spaced approximately 1.9 cm apart. It is noted that in additional or alternative embodiments, a plurality of coils may be provided, and each of the plurality of coils may have the same number of wraps or a different number of wraps. For example, an embodiment illustrating a body surrounded by two coils is illustrated with reference to FIG. 22, described in more detail

below. In some embodiments, each of the plurality of coils may have a different spacing between consecutive wraps. As illustrated in FIG. 3C, the coil may be coupled to an I/O interface (e.g., I/O interface 118 of FIG. 1). The I/O interface may communicatively couple the coil to a signal generator/receiver (e.g., one of signal generator/receivers 138 of FIG. 1 or one of the signal generator/receivers 120 of FIG. 1).

[0062] Referring to FIG 3D, the plurality of coils (e.g., 312a, 312b, and 312c) may each have a different radius. The plurality of coils may be arranged such that the plurality of coils each encircle the body 116, while, in alternate embodiments, the body 116 may encircle the plurality of coils. The plurality of coils may be arranged such that the coil with the largest radius will encircle the other coils in the plurality of coils. Different arrangements may be utilized by increasing or decreasing the number of coils in the plurality of coils, along with the distance from the plurality of coils to the body. The different arrangements can generate multiple signatures and may enable a more accurate identification of the material undergoing interrogation, such as to rule out known signatures that do not exhibit similar behaviors at a particular arrangement used to interrogate an unknown material and/or to identify known signatures that exhibit similar behaviors at a particular arrangement used to interrogate an unknown material. The parameters for a certain material determined at an arrangement may be used to cross check the parameters found in the material at other arrangements in order to generate more signatures. Generating more signatures at different arrangements may increase the reliability of material identifications performed by system 100.

[0063] Referring to FIG. 4, a flow diagram of an exemplary method for identifying an unknown material according to embodiments of the present disclosure is shown as a method 400. In some embodiments, method 400 may be stored as instructions in a memory (e.g., memory 134 of FIG. 1), and the instructions, when executed by a processor (e.g., processor 132 of FIG. 1), may cause the processor to perform the operations of method 400. At step 410, the method includes exciting one or more conductive coils with a source signal. As described above with reference to FIGs. 1-3, in some embodiments, the one or more conductive coils may surround a body defining an interior channel having a volume, and an unknown material may be retained within the volume during the interrogation/analysis. At step 420, the method includes monitoring one or more parameters associated with each of the one or more conductive coils during the exciting. As described above with reference to FIG. 1, and in more detail below with reference to FIGs. 5-20, in some embodiments, the one or more parameters associated with each of the one or more conductive coils may comprise: a

scattering parameter (e.g., one or more S11, S12, S21, S22 parameters), a resonance frequency, or a combination thereof.

[0064] In some embodiments, a frequency of the source signal used to excite the coil(s) may be between approximately 200 megahertz (MHz) and approximately 400 MHz. In
5 additional or alternative embodiments, the frequency range of the source signal may include frequencies below 200 MHz and/or frequencies above 400 MHz. In some embodiments, step 410 may further comprise varying a frequency of the source signal at which at least one of the one or more coils is excited, and step 420 may further comprise determining, during the monitoring, a resonance frequency associated with each of the one or more conductive coils.
10 In some embodiments, the resonance frequency associated with each of the one or more conductive coils may be determined at least by: setting the frequency of the source signal at which each of the one or more conductive coils is excited to each of a set of frequencies; determining, for each frequency of the set of frequencies, one or more scattering parameters associated with each of the one or more conductive coils; and identifying, as the resonance
15 frequency, the frequency of the set of frequencies at which the magnitude of scattering parameters are the smallest. For example, the source signal may be swept from a first frequency to a second frequency and one or more parameters may be observed as the frequency is swept. In some embodiments, multiple frequency sweeps may be performed, such as sweeping from the second frequency to a third frequency and one or more parameters
20 may be observed as the frequency is swept. It is noted that embodiments may sweep the frequency of the source signal two or more times, or not at all depending on a particular configuration of the interrogation system. Thus, embodiments of the present disclosure should not be limited to a particular number of frequencies or frequency sweeps that may occur during interrogation/analysis of a material.

[0065] At step 430, the method includes determining one or more signatures associated with a material within the volume based on the one or more parameters, and, at step 440, the method includes comparing the one or more signatures to one or more candidate signatures to identify the material. In some embodiments, the one or more signatures may be represented as Smith Charts. In an additional or alternative embodiment, the signatures may correspond
30 to plots of observed resonant frequencies of various scattering parameters (e.g., resonant frequencies observed based on one or more S11, S12, S21, S22, and/or the like parameters). In some embodiments, the amplitude and phase of the one or more parameters (e.g., one or more S-parameters) are measured over a range of frequencies during the monitoring (e.g., at 420), and then the one or more signatures are generated by plotting the measurements in a

Smith Chart. In some embodiments, when the measurements are plotted in the Smith Chart, the shape and location of the curve of the Smith Chart may be used to determine whether the one or more signatures of the material within the volume can be identified as a particular known material. For example, if the unknown material is purported to be milk, the Smith Chart or Smith Charts generated by interrogation of the unknown material may be compared with one or more signatures corresponding to Smith Charts generated from liquid known to be milk. Because the shape and location of the curves of different materials on the Smith Chart are different, a person may be able to identify the unknown material as milk (e.g., when the shape and location of the curves of the different Smith Charts match) or determine that the unknown material is not milk (e.g., when the shape and location of the curves of the different Smith Charts do not match). Further, in some embodiments, an electronic device (e.g., the electronic device 130 of FIG. 1) may be programmed to perform pattern recognition operations that compare the shape and location of the curve in one or more signatures of the unknown material to one or more candidate signatures (e.g., signatures of known materials). Utilizing an electronic device programmed to perform pattern recognition on the shape and location of curves present in different Smith Charts may provide a finer degree of certainty (e.g., the pattern recognition performed by the electronic device may distinguish differences that may be too subtle for the human eye to catch). This may increase the accuracy of material identifications performed in accordance with embodiments.

[0066] In some embodiments, identification of the material may indicate one or more characteristics of the material. In some embodiments, the one or more characteristics of the material may include a temperature of the material. In an additional or alternative embodiment, the one or more characteristics of the material includes a moisture content of the material. For example, where the unknown material is a soil sample, the method may be operable to determine a moisture content of the soil. The moisture content of the soil may be determined by observing the one or more parameters representative of the behavior of the coils in response to excitation (e.g., the one or more parameters may change as the moisture content of the soil changes). It is noted that in some applications of embodiments of the present disclosure, the interrogator device may not include the body. For example, where the unknown material is a soil sample, the coil(s) may be placed at a desired depth within the soil to monitor the moisture content of the soil. In such an embodiment, the coils may be coated to prevent damage to the coils. It is noted that such configurations may provide improved performance over comparable technologies suitable for performing similar applications. For example, moisture sensors for measuring soil moisture content are limited to a small area

local to the moisture sensor, whereas moisture sensors constructed according to embodiments of the present disclosure may provide for detection of soil moisture content over a much larger area, reducing the number of sensors required to cover a desired area. In another example, moisture sensors for measuring soil moisture came become inaccurate when the soil
5 has other material; other material may include but is not limited to, organic matter, other types of soil and/or air. This may provide improved performance in applications where the moisture sensors are utilized to control sprinkler systems. Additionally, the cost to deploy a soil content moisture monitoring system configured according to embodiments may be significantly lower than existing moisture sensor systems.

10 **[0067]** In an additional or alternative embodiment, the one or more characteristics of the material may indicate a solids content of the material. For example, where the material comprises a liquid and solid, the method may be operable to determine a solids content of the material. The solids content may be determined by observing the one or more parameters of a liquid and generating a signature known to be of the liquid only, and then comparing the
15 known signature to the signature of the liquid containing solid particles. Such techniques may be suitable for analysis of liquids containing nanoparticles, such as certain medications. For example, nanoparticles utilized in certain medicines must be thoroughly mixed to ensure an even distribution of the nanoparticles. The even distribution of the nanoparticles may be important for the medication to be effective, such as by ensuring that each dose contains a
20 sufficient quantity of the nanoparticles. However, if the medication is not mixed effectively, nanoparticle concentrations at the top of the liquid may be lower than nanoparticle concentrations at the bottom of the liquid. Embodiments of the present disclosure may enable a signature of a liquid containing nanoparticles that is known to have been mixed to provide an even distribution of the nanoparticles to be generated. Subsequent mixtures of the
25 liquid may be interrogated according to embodiments and the signature of the subsequent mixtures may be compared to the signature of the sufficiently mixed liquid to determine whether the subsequent mixtures comprise an even distribution of the nanoparticles. For example, mixtures comprising an uneven distribution of nanoparticles may exhibit different signatures than the mixture comprising the even distribution of the nanoparticles.

30 **[0068]** In an additional or alternative embodiment, the one or more characteristics of the material may indicate a plasma content of the material. For example, where the material comprises blood, the method may be operable to determine a plasma content of the blood. For example, samples of blood containing different plasma concentrations may exhibit different signatures when analyzed using method 400. Signatures of samples of blood

containing an unknown plasma concentration may be compared to samples of blood containing known plasma concentrations to determine the plasma concentration of the unknown samples. Additionally or alternatively, embodiments may be utilized to determine whether blood is suitable for use in medical procedures. For example, donated blood is generally believed to have a particular shelf-life when stored under particular storage conditions, and after the particular shelf-life has passed, the blood is either disposed of or expensive and time consuming chemical processes must be performed to see if the blood is suitable for use in a medical procedure. Embodiments of the present disclosure may enable donated blood to be interrogated at the time the blood is stored to generate a signature for that particular blood, and when the blood is to be used, the blood could be interrogated a second time and the signature generated during the second interrogation may be compared to the signature generated when the blood was initially stored. If the signatures match, or match to within a threshold tolerance, the blood may be determined suitable for use in a medical procedure without requiring the costly and time consuming chemical analysis. This may enable blood to be stored for longer than the particular shelf-life presently utilized today, which may help ease the demand for blood donations and increase the supply of blood available for medical procedures. Further, the interrogation provided by embodiments of the present disclosure may be performed quickly (e.g., within a few seconds), allowing the determination that the blood is suitable for medical use to be performed quickly.

[0069] In an additional or alternative embodiment, the one or more characteristics of the material may be used to identify a liquid. For example, as described in more detail below, a device operating in accordance with the method has been demonstrated to be operable to identify unknown liquids containing water, alcohol, coffee, a soft drink, milk, oil, blood, or a combination thereof. Identification of liquids may provide useful applications in many industries. For example, at airports, mothers often try to bring breastmilk onto an airplane, but are forced to throw the breastmilk out when passing through airport security. Embodiments of the present disclosure enable a signature for milk to be generated, and then the signature known to be milk may be compared to a signature generated from a sample of breastmilk in order to confirm that the sample is indeed breastmilk. In some embodiments, the breastmilk may be required to be in a specialized container specially purposed for being analyzed by an interrogation system configured according to embodiments. This allows the sample to be interrogated non-intrusively, allowing the breastmilk to remain suitable for feeding a child (e.g., the container does not need to be opened during the analysis). Further, as described below, embodiments enable identification of whether a liquid, such as milk, has

been diluted with another liquid. Thus, the analysis techniques of embodiments are sophisticated enough to detect attempts to conceal one type of liquid in another type of liquid, such as milk. Additional aspects of methods for interrogating and identifying an unknown material in accordance with embodiments of the present disclosure are illustrated and described below with reference to FIGs. 23-30.

[0070] Referring to FIG. 5, a graph illustrating various characteristics of different liquids that have been interrogated according to embodiments of the present disclosure is shown. As illustrated in FIG. 5, S-parameters, and in particular the S_{11} parameter, have different minimum peaks for different liquids. For example, in FIG. 5, minimum peaks for deionized (DI) water 510, alcohol 520, coffee 530, a soda 540, milk 550, a sports drink 560, and vodka 570 are shown. As illustrated in FIG. 5, each of these liquids exhibits a minimum peak that is distinguishable from the minimum peaks of the other liquids in terms of the frequency at which the S_{11} minimum peak occurs and/or the magnitude of the minimum peak. During interrogation of an unknown liquid according to embodiments of the present disclosure, an unknown liquid may be identified as one of the listed types of liquids by observing the minimum S_{11} peak at different frequencies.

[0071] For example, the unknown liquid may be placed within volume 114 of interrogator device 110 and coil(s) 112 may be excited at one or more frequencies by the signal generator/receiver 138 of the electronic device 130. signal generator/receiver 138 of electronic device 130 may monitor the behavior of coil(s) 112 during the excitement to determine one or more parameters, such as one or more S-parameters, representative of coil(s) 112 during the excitement. If the one or more determined parameters includes an S_{11} min peak having a magnitude of approximately 0.11 at an interrogation frequency of approximately 2.71, the unknown liquid likely contains a soda drink, such as soda drink 540, and electronic device 130 of FIG. 1 may identify the liquid as containing a soda drink. In some embodiments, the liquid may be identified as containing a soda drink by creating a signature based on the observed parameters, and then compare the signature observed during interrogation of the unknown liquid (e.g., during the exciting of coil(s) 112 by signal generator/receiver 138) to one or more signatures of known liquids to determine whether the signature generated based on parameters observed during interrogation of the unknown liquid matches any of the one or more signatures of the known liquids. In some embodiments, the one or more signatures of the known liquids may be stored in a database (e.g., as known characteristic data 142 at database 140 of FIG. 1). It is noted that the liquid identification techniques of embodiments are capable of identifying additional liquids than those shown in

FIG. 5, and that the liquids and their corresponding minimum |S₁₁| peaks are shown for purposes of illustration, rather than by way of limitation.

[0072] Referring to FIG. 6, a chart illustrating characteristics observed during interrogation of liquids containing alcohol at different concentrations according to 5 embodiments of the present disclosure are shown. In some embodiments, the information illustrated in FIG. 6 was observed using the system 100 of FIG. 1 and illustrates a plot of values representing the log magnitude for various observed values of an S-parameter (e.g., S₁₁) during interrogation of a liquid by a device configured according to the embodiment illustrated in FIG. 1, as described in more detail below. For example, liquids containing 10 different concentrations of alcohol may be placed within volume 114 of interrogator device 110 and coil(s) 112 may be excited at one or more frequencies by signal generator/receiver 138 of electronic device 130. Signal generator/receiver 138 of electronic device 130 may monitor the behavior of coil(s) 112 during the excitement to determine one or more parameters, such as one or more S-parameters, representative of coil(s) 112 during the 15 excitement, as described above with reference to FIGs. 1-4. In FIG. 6, observed |S₁₁| values for various concentrations of alcohol are shown at a range of frequencies (e.g., from approximately 2 Hz to approximately 4Hz). The various concentrations of alcohol include a 5% concentration of alcohol 610, a 15% concentration of alcohol 620, a 25% concentration of alcohol 630, a 50% concentration of alcohol 640, a 75% concentration of alcohol 650, a 20 100% concentration of alcohol 660. As shown at box 602, minimum |S₁₁| peaks for the different concentrations of alcohol 610-660 are observed at frequencies of approximately 2.7-2.8 Hz and have an |S₁₁| magnitude ranging from approximately 0.1 to 0.27. In some embodiments, this information may be used to generate one or more signatures that may be stored (e.g., as part of known characteristic data 142 of FIG. 1) at a database (e.g., database 25 140 of FIG. 1). Once stored, these signatures may be compared to signatures of an unknown liquid to determine whether the liquid contains alcohol at one of the various concentrations illustrated in FIGs. 6-9.

[0073] Referring to FIG. 7, a diagram illustrating a plot of resonant frequencies observed during interrogation of liquids containing alcohol at different concentrations is shown. In 30 some embodiments, the information illustrated in FIG. 7 was generated based on information observed using system 100 of FIG. 1 (e.g., placing liquids containing different concentrations of alcohol within volume 114 of interrogator device 110, exciting coil(s) 112 at one or more frequencies by signal generator/receiver 138 of electronic device 130, and monitoring the behavior of coil(s) 112 during the excitement to determine one or more parameters). In some

embodiments, the points plotted in FIG. 7 correspond to the different concentrations of alcohol illustrated with reference to FIG. 6. In some embodiments, the resonant frequencies illustrated in FIG. 7 may be utilized to generate signatures representative of the various concentrations of alcohol and the signatures generated based on the resonant frequency data
5 illustrated in FIG. 7 may be stored (e.g., as part of known characteristic data 142 of FIG. 1) at a database (e.g., database 140 of FIG. 1). Once stored, these signatures may be compared to signatures of an unknown liquid to determine whether the liquid contains alcohol at one of the various concentrations illustrated in FIGs. 6-9.

[0074] Referring to FIG. 8, a diagram illustrating a plot of the minimum |S₁₁| peaks
10 observed during interrogation of liquids containing alcohol at different concentrations is shown. In some embodiments, the information illustrated in FIG. 8 was generated based on information observed using system 100 of FIG. 1 (e.g., placing liquids containing different concentrations of alcohol within volume 114 of interrogator device 110, exciting coil(s) 112 at one or more frequencies by signal generator/receiver 138 of electronic device 130, and
15 monitoring the behavior of coil(s) 112 during the excitement to determine one or more parameters). As illustrated in FIG. 8, a liquid containing an approximately 5% concentration of alcohol will exhibit a minimum |S₁₁| peak having a magnitude of approximately 0.25 at a frequency of approximately 2.69 Hz, a liquid containing an approximately 15% concentration of alcohol will exhibit a minimum |S₁₁| peak having a magnitude of approximately 0.24 at a
20 frequency of approximately 2.7 Hz, a liquid containing an approximately 25% concentration of alcohol will exhibit a minimum |S₁₁| peak having a magnitude of approximately 0.22 at a frequency of approximately 2.69 Hz, a liquid containing an approximately 50% concentration of alcohol will exhibit a minimum |S₁₁| peak having a magnitude of approximately 0.19 at a frequency of approximately 2.72 Hz, a liquid containing an approximately 75% concentration
25 of alcohol will exhibit a minimum |S₁₁| peak having a magnitude of approximately 0.15 at a frequency of approximately 2.71 Hz, and a liquid containing an approximately 100% concentration of alcohol will exhibit a minimum |S₁₁| peak having a magnitude of approximately 0.06 at a frequency of approximately 2.78 Hz. In some embodiments, the minimum |S₁₁| peaks illustrated in FIG. 8 may be utilized to generate signatures
30 representative of the various concentrations of alcohol and the signatures generated based on the resonant frequency data illustrated in FIG. 8 may be stored (e.g., as part of known characteristic data 142 of FIG. 1) at a database (e.g., database 140 of FIG. 1). Once stored, these signatures may be compared to signatures of an unknown liquid to determine whether the liquid contains alcohol at one of the various concentrations illustrated in FIGs. 6-9.

[0075] Referring to FIG. 9, a diagram illustrating Smith charts generated based on observations during interrogation of liquids containing alcohol at different concentrations is shown. In some embodiments, the information illustrated in FIG. 9 was generated based on information observed using system 100 of FIG. 1. As illustrated in FIG. 9, each of the different concentrations of alcohol is uniquely represented on a Smith chart, and the resonant frequencies (e.g., the resonant frequencies illustrated in FIG. 7) are illustrated as circles having labels corresponding to their counterpart concentrations with an “r” appended to the end of the label (e.g., the circle 610r represents the resonant frequency corresponding to a 5% concentration of alcohol 610, etc.). In some embodiments, the various Smith charts for each concentration of alcohol illustrated in FIG. 9 may be utilized to generate signatures representative of the various concentrations of alcohol, and the signatures generated based on the Smith charts illustrated in FIG. 9 may be stored (e.g., as part of known characteristic data 142 of FIG. 1) at a database (e.g., database 140 of FIG. 1). Once stored, these signatures may be compared to signatures of an unknown liquid to determine whether the liquid contains alcohol at one of the various concentrations illustrated in FIGs. 6-9. As shown in FIG. 9, Smith chart 660 corresponding to a sample of pure alcohol can be visually distinguished from samples of alcohol that have been diluted. In some embodiments, when determining whether a liquid purported to be alcohol is analyzed, a Smith chart known to be generated from pure alcohol and a Smith chart of the sample purported to be alcohol may be displayed at a display device, and an operator may be able to determine whether the sample is what it is purported to be simply by viewing the displayed Smith charts. In additional or alternative embodiments, a system, such as the system 100 of FIG. 1, may compare the Smith charts and provide an output that indicates whether the sample is what it is purported to be.

[0076] Referring to FIG. 10, a chart illustrating characteristics observed during interrogation of liquids containing milk at different concentrations according to embodiments of the present disclosure are shown. In some embodiments, the information illustrated in FIG. 6 was observed using the system 100 of FIG. 10 and illustrates a plot of values representing the log magnitude for various observed values of an S-parameter (e.g., S₁₁) during interrogation of a liquid by a device configured according to the embodiment illustrated in FIG. 1, as described in more detail below. For example, liquids containing different concentrations of milk may be placed within volume 114 of interrogator device 110 and coil(s) 112 may be excited at one or more frequencies by signal generator/receiver 138 of electronic device 130. Signal generator/receiver 138 of electronic device 130 may monitor the behavior of coil(s) 112 during the excitement to determine one or more parameters, such

as one or more S-parameters, representative of coil(s) 112 during the excitement, as described above with reference to FIGs. 1-4. In FIG. 10, observed IS111 values for various concentrations of milk are shown at a range of frequencies (e.g., from approximately 2 Hz to approximately 4Hz). In some embodiments, the information illustrated in FIG. 10 was
5 observed using system 100 of FIG. 1. The various concentrations of milk include a 5% concentration of milk 1010, a 15% concentration of milk 1020, a 25% concentration of milk 1030, a 50% concentration of milk 1040, a 75% concentration of milk 1050, a 100% concentration of milk 1060. As shown at box 1002, minimum IS111 peaks for the different concentrations of milk 1010-1060 are observed at frequencies of approximately 2.6-2.7 Hz
10 and have an IS111 magnitude ranging from approximately 0.03 to 0.2. In some embodiments, this information may be used to generate one or more signatures that may be stored (e.g., as part of known characteristic data 142 of FIG. 1) at a database (e.g., database 140 of FIG. 1). Once stored, these signatures may be compared to signatures of an unknown liquid to determine whether the liquid contains milk at one of the various concentrations illustrated in
15 FIGs. 10-13.

[0077] Referring to FIG. 11, a diagram illustrating a plot of resonant frequencies observed during interrogation of liquids containing milk at different concentrations is shown. In some embodiments, the information illustrated in FIG. 11 was generated based on information observed using system 100 of FIG. 1 (e.g., placing liquids containing different
20 concentrations of milk within volume 114 of interrogator device 110, exciting coil(s) 112 at one or more frequencies by signal generator/receiver 138 of electronic device 130, and monitoring the behavior of coil(s) 112 during the excitement to determine one or more parameters). In some embodiments, the points plotted in FIG. 11 correspond to the different concentrations of milk illustrated with reference to FIG. 10. In some embodiments, the resonant frequencies illustrated in FIG. 11 may be utilized to generate signatures
25 representative of the various concentrations of milk and the signatures generated based on the resonant frequency data illustrated in FIG. 11 may be stored (e.g., as part of known characteristic data 142 of FIG. 1) at a database (e.g., database 140 of FIG. 1). Once stored, these signatures may be compared to signatures of an unknown liquid to determine whether
30 the liquid contains milk at one of the various concentrations illustrated in FIGs. 10-13.

[0078] Referring to FIG. 12, a diagram illustrating a plot of the minimum IS111 peaks observed during interrogation of liquids containing milk at different concentrations is shown. In some embodiments, the information illustrated in FIG. 12 was generated based on information observed using system 100 of FIG. 1 (e.g., placing liquids containing different

concentrations of milk within volume 114 of interrogator device 110, exciting coil(s) 112 at one or more frequencies by signal generator/receiver 138 of electronic device 130, and monitoring the behavior of coil(s) 112 during the excitement to determine one or more parameters). As illustrated in FIG. 12, a liquid containing an approximately 5% concentration of milk 1010 will exhibit a minimum |S11| peak having a magnitude of approximately 0.21 at a frequency of approximately 2.68 Hz, a liquid containing an approximately 15% concentration of milk 1020 will exhibit a minimum |S11| peak having a magnitude of approximately 0.28 at a frequency of approximately 2.65 Hz, a liquid containing an approximately 25% concentration of milk 1030 will exhibit a minimum |S11| peak having a magnitude of approximately 0.15 at a frequency of approximately 2.67 Hz, a liquid containing an approximately 50% concentration of milk 1040 will exhibit a minimum |S11| peak having a magnitude of approximately 0.14 at a frequency of approximately 2.69 Hz, a liquid containing an approximately 75% concentration of milk 1050 will exhibit a minimum |S11| peak having a magnitude of approximately 0.33 at a frequency of approximately 2.64 Hz, and a liquid containing an approximately 100% concentration of milk 1060 will exhibit a minimum |S11| peak having a magnitude of approximately 0.46 at a frequency of approximately 2.68 Hz. In some embodiments, the minimum |S11| peaks illustrated in FIG. 12 may be utilized to generate signatures representative of the various concentrations of milk and the signatures generated based on the resonant frequency data illustrated in FIG. 12 may be stored (e.g., as part of known characteristic data 142 of FIG. 1) at a database (e.g., database 140 of FIG. 1). Once stored, these signatures may be compared to signatures of an unknown liquid to determine whether the liquid contains milk at one of the various concentrations illustrated in FIGs. 10-13.

[0079] Referring to FIG. 13, a diagram illustrating Smith charts generated based on observations during interrogation of liquids containing milk at different concentrations is shown. In some embodiments, the information illustrated in FIG. 13 was generated based on information observed using system 100 of FIG. 1 (e.g., placing liquids containing different concentrations of milk within volume 114 of interrogator device 110, exciting coil(s) 112 at one or more frequencies by signal generator/receiver 138 of electronic device 130, and monitoring the behavior of coil(s) 112 during the excitement to determine one or more parameters). As illustrated in FIG. 13, each of the different concentrations of milk is uniquely represented on a Smith chart, and the resonant frequencies (e.g., the resonant frequencies illustrated in FIG. 11) are illustrated as circles having labels corresponding to their counterpart concentrations with an “r” appended to the end of the label (e.g., the circle

1010r represents the resonant frequency corresponding to a 5% concentration of milk 1010, etc.). In some embodiments, the various Smith charts for each concentration of milk illustrated in FIG. 13 may be utilized to generate signatures representative of the various concentrations of milk and the signatures generated based on the Smith charts illustrated in 5 FIG. 13 may be stored (e.g., as part of known characteristic data 142 of FIG. 1) at a database (e.g., database 140 of FIG. 1). Once stored, these signatures may be compared to signatures of an unknown liquid to determine whether the liquid contains milk at one of the various concentrations illustrated in FIGs. 10-13. As shown in FIG. 13, Smith chart 1060 corresponding to a sample of pure milk can be visually distinguished from samples of milk 10 that have been diluted. In some embodiments, when determining whether a liquid purported to be milk is analyzed, a Smith chart known to be generated from pure milk and a Smith chart of the sample purported be milk may be displayed at a display device, and an operator may be able to determine whether the sample is what it is purported to be simply by viewing the displayed Smith charts. In additional or alternative embodiments, a system, such as system 15 100 of FIG. 1, may compare the Smith charts and provide an output that indicates whether the sample is what it is purported to be.

[0080] Referring to FIG. 14, a chart illustrating characteristics observed during interrogation of liquids containing different milk/alcohol mixes according to embodiments of the present disclosure is shown. In some embodiments, the information illustrated in FIG. 6 20 was observed using the system 100 of FIG. 14 and illustrates a plot of values representing the log magnitude for various observed values of an S-parameter (e.g., S₁₁) during interrogation of a liquid by a device configured according to the embodiment illustrated in FIG. 1, as described in more detail below. For example, liquids containing different milk and alcohol percentages may be placed within volume 114 of interrogator device 110 and coil(s) 112 may 25 be excited at one or more frequencies by signal generator/receiver 138 of electronic device 130. Signal generator/receiver 138 of electronic device 130 may monitor the behavior of coil(s) 112 during the excitement to determine one or more parameters, such as one or more S-parameters, representative of coil(s) 112 during the excitement, as described above with reference to FIGs. 1-4. In FIG. 14, observed |S₁₁| values for liquids containing various milk 30 and alcohol percentages are shown at a range of frequencies (e.g., from approximately 2 Hz to approximately 4Hz). As shown in FIG. 14, the magnitude of the observed minimum |S₁₁| peaks ranged from approximately 0.02 to approximately 0.08, as shown in box 1402, and occur approximately between 2.6 Hz and 2.8 Hz. As illustrated in FIG. 14, a liquid containing a 5% milk/alcohol mix is represented at 1410, a liquid containing a 15%

milk/alcohol mix is represented at 1420, a liquid containing a 25% milk/alcohol mix is represented at 1430, a liquid containing a 50% milk/alcohol mix is represented at 1440, a liquid containing a 75% milk/alcohol mix is represented at 1450, and a liquid containing a 100% milk/alcohol mix is represented at 1460.

5 **[0081]** Referring to FIG. 15, a diagram illustrating a plot of resonant frequencies observed during interrogation of liquids containing different milk/alcohol mixes according to embodiments is shown. In some embodiments, the information illustrated in FIG. 15 was generated based on information observed using system 100 of FIG. 1 (e.g., placing liquids containing different milk/alcohol mixes within volume 114 of interrogator device 110,
10 exciting coil(s) 112 at one or more frequencies by signal generator/receiver 138 of electronic device 130, and monitoring the behavior of coil(s) 112 during the excitement to determine one or more parameters). In some embodiments, the points plotted in FIG. 15 correspond to, and represent the resonant frequencies of, the liquids of different milk/alcohol mixes illustrated with reference to FIG. 14. In some embodiments, the resonant frequencies
15 illustrated in FIG. 15 may be utilized to generate signatures representative of the various liquids containing the different milk/alcohol mixes. These signatures may then be compared against signatures of liquids containing known milk/alcohol mixes to identify the components of the liquids under observation (e.g., identify liquids containing particular milk/alcohol mixes).

20 **[0082]** Referring to FIG. 16, a diagram illustrating a plot of the minimum |S₁₁| peaks observed during interrogation of liquids containing different milk/alcohol mixes is shown. In some embodiments, the information illustrated in FIG. 16 was generated based on information observed using system 100 of FIG. 1 (e.g., placing liquids containing different milk/alcohol mixes within volume 114 of interrogator device 110, exciting coil(s) 112 at one
25 or more frequencies by signal generator/receiver 138 of electronic device 130, and monitoring the behavior of coil(s) 112 during the excitement to determine one or more parameters). As illustrated in FIG. 16, a liquid containing an approximately 5% concentration of milk/alcohol mix 1410 will exhibit a minimum |S₁₁| peak having a magnitude of approximately 0.18 at a frequency of approximately 2.66 Hz, a liquid
30 containing an approximately 15% concentration of milk/alcohol mix 1420 will exhibit a minimum |S₁₁| peak having a magnitude of approximately 0.15 at a frequency of approximately 2.67 Hz, a liquid containing an approximately 25% concentration of milk/alcohol mix 1430 will exhibit a minimum |S₁₁| peak having a magnitude of approximately 0.16 at a frequency of approximately 2.66 Hz, a liquid containing an

approximately 50% concentration of milk/alcohol mix 1050 will exhibit a minimum |S₁₁| peak having a magnitude of approximately 0.14 at a frequency of approximately 2.69 Hz, a liquid containing an approximately 75% concentration of milk 1050 will exhibit a minimum |S₁₁| peak having a magnitude of approximately 0.33 at a frequency of approximately 2.64 Hz, and a liquid containing an approximately 100% concentration of milk 1060 will exhibit a minimum |S₁₁| peak having a magnitude of approximately 0.46 at a frequency of approximately 2.68 Hz. In some embodiments, the minimum |S₁₁| peaks illustrated in FIG. 16 may be utilized to generate signatures representative of the various milk/alcohol mixes and the signatures may be stored (e.g., as part of known characteristic data 142 of FIG. 1) at a database (e.g., database 140 of FIG. 1). Once stored, these signatures may be compared to signatures of an unknown liquid to determine whether the liquid contains a milk/alcohol mixture corresponding to one of the various milk/alcohol mixes illustrated in FIGs. 14-17.

[0083] Referring to FIG. 17, a diagram illustrating Smith charts generated based on observations during interrogation of liquids containing different milk/alcohol mixes is shown. In some embodiments, the information illustrated in FIG. 17 was generated based on information observed using system 100 of FIG. 1 (e.g., placing liquids containing different milk/alcohol mixes within volume 114 of interrogator device 110, exciting coil(s) 112 at one or more frequencies by signal generator/receiver 138 of electronic device 130, and monitoring the behavior of coil(s) 112 during the excitement to determine one or more parameters). As illustrated in FIG. 17, each of the different milk/alcohol mixes is uniquely represented on a Smith chart, the resonant frequencies (e.g., the resonant frequencies illustrated in FIG. 15 that are the frequencies when the S-parameter curves pass the horizontal axis) and the S-parameter locations at the original resonant frequency of 272 MHz, which are illustrated as circles having labels corresponding to their counterpart concentrations with an “r” appended to the end of the label (e.g., the circle 1410r represents the resonant frequency corresponding to a 5% milk/alcohol mixes 1410, etc.). As shown in FIGs. 15-17, the resonant frequency observed for milk shifts as the concentration of alcohol in the milk/alcohol mix increases. This can be observed by comparing the resonant frequency of milk illustrated by the curve 1760 of FIG. 17 (e.g., the resonating frequency of a milk in a mixture containing 50% milk and 50% alcohol) with the resonating frequency represented by the curve 1770 (e.g., the resonating frequency of a 100% concentration of milk) of FIG. 17. Comparing the locations of the circle 1770r (e.g., the resonating frequency of a milk in a mixture containing 100% milk) with the locations of the same frequency of 272 MHz on the Smith Chart may be used to identify the liquid content. In some embodiments,

the various Smith Charts for each milk/alcohol mix illustrated in FIG. 17 may be utilized to generate signatures representative of the various milk/alcohol mixes and the signatures generated based on the shape of the Smith Chart curves illustrated in FIG. 17 may be stored (e.g., as part of known characteristic data 142 of FIG. 1) at a database (e.g., database 140 of FIG. 1). Once stored, these signatures may be compared to signatures of an unknown liquid to determine whether the liquid contains a milk/alcohol mix corresponding to one of the mixes illustrated with reference to FIGs. 14-17.

[0084] Referring to FIG. 18A, a diagram illustrating aspects of an embodiment of the present sample-interrogators comprising a plurality of coils according to the present disclosure is shown. In FIG. 18A, body 222 of FIG. 2 is shown, and, as described above with reference to FIGs. 1 and 2, the body 222 may define an interior channel or opening that provides a volume, such as volume 214 of FIG. 2. In the particular embodiment illustrated in FIG. 18A, body 222 has a height of approximately 9.7 centimeters (cm) and a diameter of approximately 4.2 cm. A first coil 1810 and a second coil 1820 may be provided, and each of the coils 1810, 1820 may surround the body 222. For example, and referring briefly to FIG. 21, a diagram illustrating an embodiment of an interrogator device having a body surrounded by two coils is shown. As illustrated in FIG. 21, the different coils may comprise a different number of wraps (e.g., may wrap around body 222 a different number of times), and may have a different spacing between wraps. It is noted however, that the particular configuration of coils 1810, 1820 shown in FIG. 21 is provided for purposes of illustration, rather than by way of limitation, and in some embodiments, more than two coils may be used, a plurality of coils with the same number of wraps with the same or different spacing between two or more of the plurality of coils may be used, or other configurations depending on a particular purpose or configuration of the interrogation device. Thus, embodiments of the present disclosure are not to be limited to a particular number of coils, a particular number of wraps, or a particular spacing between wraps.

[0085] Additionally, as shown in FIG. 21, each of the coils may provide a port. The port may provide an I/O interface for coupling the coils to an interrogation device, such as electronic device 130 of FIG. 1 which includes the one or more signal generators/receivers 138. Signal generator(s)/receiver(s) 138 may provide a respective source signal to each of coils 1810, 1820 via the respective ports to excite the coils, and may measure one or more parameters characteristic of the behavior of coils 1810, 1820 in response to the exciting of the coils, such as scattering parameters with representative reflection coefficients (e.g., S11 and S22 parameters), and transmission coefficients (e.g., S12 and S21), and resonance

frequencies, the curve shapes and locations on the Smith Chart, or a combination thereof for each of coils 1810, 1820. These parameters may be used to generate signatures that may be stored in a database (e.g., database 140 of FIG. 1) as either sample data 144 (e.g., when the liquid within volume 214 is an unknown liquid to be identified) or known characteristics data
5 142 (e.g., when liquid within volume 214 is a known liquid or mixture of liquids).

[0086] In a similar embodiments to the interrogator having a plurality of coils as shown in FIG 18, an alternative embodiment may include a plurality of coils such that each coil is positioned at a different lateral distance from a body 222. Alternatively, one or more single strip antenna(e) may be used in combination or as a replacement for the coils 112. Referring
10 to FIG 3D, the plurality of coils (e.g., 1812a, 1812b, and 1812c) may have a different radius than the rest of the plurality of coils. The plurality of coils may be arranged such that the plurality of coils each encircle the body 222, while, in alternate embodiments, the body 222 may encircle the plurality of coils. The plurality of coils may be arranged such that the coil with the largest radius will encircle the other coils in the plurality of coils. Different
15 arrangements may be utilized by increasing or decreasing the number of coils in the plurality of coils, along with the distance from the plurality of coils to the body. As described in more detail above, signal generator(s)/receiver(s) may provide a signal to excite the coils, and may measure one or more parameters of the coils to generate signatures that can be stored in a database. It is noted however, that the particular configuration of coils 1812a, 1812b, and
20 1812c shown in FIG. 18B is provided for purposes of illustration, rather than by way of limitation, and in some embodiments, more or less than three coils may be used, a plurality of coils with the same or different spacing between the plurality of coils may be used, or other configurations depending on a particular purpose or configuration of the interrogation device. Thus, embodiments of the present disclosure are not to be limited to a particular number of
25 coils or a particular spacing between coils. It is noted that in additional or alternative embodiments, a plurality of antenna(e) may be provided, and each of the plurality of antenna(e) may have a different radius and may be encircle the body in increasing distances relative to their radii. In other embodiments, the plurality of antenna(e) are encircled by the
body.

[0087] Additionally, as shown in FIG. 18B, a switch 1840 may be used to selectively activate one or more coils of the plurality of coils. For example, switch 1840 may selectively activate coil 1812a to generate a signature as described above. In another example, switch 1840 may selectively activate coils 1812a, and 1812c to generate a signature. The switch
30 may be configured such that it can selectively activate and deactivate any coil in the plurality

of coils to act individually or in combination with any other coil(s) in the plurality of coils. In some embodiments, not pictured, phase matching the plurality of coils may occur. In some embodiments a matching circuit may be coupled in series with the coil(s). The matching circuit may be used to match the impedance between two points of the interrogator device

5 100, such that power transfer is optimized to the coil(s) 112. Optimizing power transfer to the coils(s) 112 may increase the sensitivity of the signatures by generating more precise parameters. For example, a Pi matching circuit may be used to generate higher quality factors in resonance when identifying de-ionized water. The matching circuit may enhance sensitivity to other parameters used by the interrogator 100, as described in more detail below

10 **[0088]** Referring back to FIG. 18A, as illustrated at 1830 and 1840, each of coils 1810 may have multiple resonant frequencies, shown at 1830 with respect to first coil 1810 and 1840 with respect to second coil 1820. As shown in FIG. 18A, first coil 1810 may have resonant frequencies at f_{011} and f_{012} , as shown at 1830, and second coil 1820 may have resonant frequencies at f_{021} and f_{022} , as shown at 1840 when the known material is

15 deionized water. One or more signatures may be generated based on these observed parameters, and then those signatures may be used to identify an unknown liquid (e.g., determine whether the unknown liquid is deionized water). For example, and referring to FIGs. 19 and 20, when an unknown liquid is interrogated using the coil configuration illustrated in FIG. 18A, the first coils 1810 may have resonant frequencies 1834 and the

20 second coil 1820 may have resonant frequencies of 1844. As shown in FIGs. 19 and 20, when the unknown liquid is interrogated, the resonant frequencies of the coil 1810 illustrated at 1834 may be shifted by f_{11} and f_{12} relative to those of 1832 (e.g., the resonant frequencies of the first coil 1810 as observed during interrogation of DI water), and the resonant frequencies of the coil 1820 illustrated at 1844 may be shifted by f_{21} and f_{22} relative to those

25 of 1842 (e.g., the resonant frequencies of the second coil 1820 as observed during interrogation of DI water). In some embodiments, these frequency shifts and the corresponding magnitudes of the S-parameters at the resonant frequencies may be used to identify the unknown liquid by comparing this data to information stored in a database (e.g., the database 140 of FIG. 1). In some embodiments, the comparison of the frequency shifts and corresponding magnitudes of the S-parameters at the resonant frequencies may be

30 performed using Smith Charts, as described below with reference to FIG. 22.

[0089] Referring to FIG. 22, a diagram illustrating an embodiment of an additional technique for identifying an unknown liquid according to the present disclosure is shown. In some embodiments, the Smith Charts illustrates in FIG. 22 may be generated using an

interrogation device configured according to the embodiments illustrated with reference to FIGs. 18A and 21 (e.g., an interrogation device comprising two coils, such as the coils 1810 and 1820 of FIGs. 18A and 21). In FIG. 22, a first Smith chart 2210, a second Smith chart 2220, a third Smith chart 2230, a fourth Smith chart 2240 are shown. First Smith chart 2210
5 may represent the resonant frequency observed at f_{011} during excitement of first coil 1810 and/or second coil 1820 of FIG. 18A, second Smith chart 2220 may represent the resonant frequency observed at f_{012} during excitement of first coil 1810 and/or second coil 1820 of FIG. 18A, third Smith chart 2230 may represent the resonant frequency observed at f_{021} during excitement of first coil 1810 and/or second coil 1820 of FIG. 18A, and fourth Smith
10 chart 2240 may represent the resonant frequency observed at f_{022} during excitement of first coil 1810 second coil 1820 of FIG. 18A. In some embodiments, f_{012} may depend on or be effected by excitation of coil 2, and/or f_{021} may depend on or be effected by excitation of coil 1. In some embodiments, Smith charts associated with the resonant frequencies observed during interrogation of an unknown liquid may be compared to the Smith charts illustrated in
15 FIG. 22 to identify the unknown liquid. If the shapes and locations of the curves in the Smith Charts and/or resonant frequencies match to within a threshold tolerance, the unknown liquid may be identified as the known liquid used to produce Smith charts 2210-2240. If the shapes and locations of the curves in the Smith charts and/or resonant frequencies generated for the unknown liquid do not match Smith charts 2210-2240 to within the threshold tolerance, the
20 Smith charts generated for the unknown liquid may be compared to Smith charts generated for additional known liquids to identify the unknown liquid. Embodiments utilizing a plurality of coils, such as the embodiments described with reference to FIGs. 18-22, may provide improved accuracy when identifying unknown liquids. For example, using two coils may enable more features or parameters to be observed during interrogation of the liquid,
25 providing more points of comparison for signature identification and matching purposes.

[0090] Referring to FIG. 23, charts illustrating characteristics observed during interrogation of a material using coil(s) according to the present disclosure are shown. In some embodiments, the charts illustrated in FIG. 23 may be generated using an interrogation device configured according to the embodiment illustrated in FIG. 18B (e.g., an interrogation
30 devices having three coils each encircling the body and a switch configured to selectively activate the coil(s)). In FIG. 23, a first chart 2310, a second chart 2320, a third chart 2330, and a fourth chart 2340 are shown, where each chart represents a different arrangement of coils in the system. The charts may display the plot of various observed parameter values (e.g., values of an S-parameter— S_{11}) during interrogation of a liquid across a range of

frequencies (e.g., from approximately 300 MHz to 600 MHz). First chart 2310 may represent the S11 parameters observed during interrogation of a liquid at an arrangement using the coil 1812a of FIG 18B. Second chart 2320 may represent the S11 parameters observed during interrogation of a liquid at an arrangement using the coil 1812b of FIG 18B. Third chart 2330 may represent the S11 parameters observed during interrogation of a liquid at an arrangement using the coil 1812c of FIG 18B. Forth chart 2340 may represent the S11 parameters observed during interrogation of a liquid at an arrangement using coil 1812b and 1812c of FIG 18B. As described above, parameters may be observed at one or more frequencies during interrogation. In some embodiments the use of switch 1840, of FIG 18B, may allow generation of multiple charts possible without removal or reconfiguration of the interrogator. The interrogation may be performed for several liquids using each arrangement of the interrogator. For example, liquids containing different alcohol percentages may be placed within the interrogator device and the measured parameters of each liquid may be charted for each arrangement. More specifically, DI water 2302, may be plotted with several other liquids containing alcohol (50% alcohol 2304, 100% alcohol 2306, and gasoline 2308). As FIG. 23 shows, the resonant frequencies for each liquid can be distinguished by the interrogator using the methods described above for each arrangement 2310, 2320, 2330, and 2340. In other embodiments, characteristics observed during interrogation may also be configured to display Smith charts

[0091] Referring to FIG. 24, charts illustrating characteristics observed during interrogation of a material using a plurality of coils according to the present disclosure are shown. In some embodiments the charts illustrated in FIG. 24 may be generated using an interrogation device configured according to the embodiment illustrated in FIG. 18B (e.g., an interrogation devices having three coils each encircling the body). In FIG. 24 a first chart 2410 and a second chart 2420 are shown. First chart 2410 may represent the S11 parameters observed during interrogation of a liquid at an arrangement using the plurality of coils 1812a, 1812b and 1812c of FIG 18B. In some embodiments phase matching may be used to increase the sensitivity of the coils. Second chart 2420 may represent the S11 parameters observed during interrogation of a liquid at an arrangement using the plurality of coils 1812a, 1812b and 1812c of FIG 18B using a phase matching device. For example, a pi matching circuit may be coupled in series with the sensor coils 1812a, 1812b and 1812c of FIG 18B. Phase matching may be used to increase the accuracy of the signatures generated by the interrogator. For example, a matching circuit may improve the S11 parameters, thus improving the signatures, by generating high quality factors when using multiple coils.

[0092] The different arrangements of the plurality of coils can generate multiple signatures and may enable a more accurate identification of the material undergoing interrogation, such as to rule out known signatures that do not exhibit similar behaviors at a particular arrangement used to interrogate an unknown material and/or to identify known signatures that exhibit similar behaviors at a particular arrangement used to interrogate an unknown material. For example, as illustrated by FIG. 25, six resonance frequencies can be generated from the six arrangements in accordance with the embodiment illustrated in FIG. 18. The new signatures may be added to the data base to increase the reliability of material identifications performed by the interrogator.

[0093] Referring to FIG 26, the parameters for a certain material determined at an arrangement may be used to cross check the parameters found in the material at other arrangements in order to generate more signatures. The parameters for a liquid measured in certain arrangements may be used as a reference point to generate signatures based on the observed parameters of other liquids in the same arrangement. For example, using the parameters found in FIG. 25, the resonant frequency of gasoline generated for all six arrangements (2310, 2320, 2330, 2340, 2410, 2420) may be set as a reference point and the relative frequency shifts of the other liquids (DI water 2302, 50% Alcohol 2304, and 100% Alcohol 2306) may be used as a signature for those arrangements.

[0094] Referring to FIG. 27, a flow diagram of exemplary method for identifying an unknown material in accordance with embodiments of the present disclosure is shown as a method 2700. In some embodiments, the method 2700 may correspond to step 440 of method 400 illustrated and described above with reference to FIG. 4. At step 2710, method 2700 includes checking for the presence of a minimum peak within a particular narrowband frequency range. At step 2720, a determination is made as to whether the minimum peak is present within a particular narrowband frequency range (e.g., a narrowband frequency range where a known material exhibits a minimum peak). If the minimum peak is present within the particular narrowband frequency range, the unknown material is identified as the material corresponding to the particular narrowband frequency range (e.g., the known material that exhibits a minimum peak at the particular narrowband frequency range), otherwise, the method 2700 continues to step 2730 where the presence of a minimum |S11| peak within a particular narrowband frequency range is checked. At step 2740, a determination is made as to whether the minimum |S11| peak is present within a particular narrowband frequency range (e.g., a narrowband frequency range where a known material exhibits a minimum |S11| peak). If the minimum |S11| peak is present within the particular narrowband frequency range, the

unknown material is identified as the material corresponding to the particular narrowband frequency range (e.g., the known material that exhibits a minimum |S11| peak at the particular narrowband frequency range), otherwise the method 2700 continues to step 2750. At step 2750, the method 2700 checks an absolute frequency range for the presence of a minimum peak, and, at step 2760, if the minimum peak is found within a particular absolute range, the material is identified. Otherwise, the material cannot be identified (e.g., because the material does not exhibit characteristics of a known material or combination of materials). In FIG. 27, a minimum peak total frequency range 2770 for various materials is shown and includes a minimum peak total frequency range for DI, alcohol, and vodka.

10 **[0095]** FIG. 28 is a diagram that illustrates additional aspects of frequency ranges that may be used to identify a material according to embodiments. For example, in FIG. 28, a minimum peak frequency narrow range 2810, a minimum |S11| peak narrow range 2820, a minimum peak frequency total range 2830, and a minimum |S11| peak total range 2840 are shown. Minimum peak frequency total range 2830 may be the same as minimum peak total frequency range 2770 illustrated in FIG. 27. Minimum peak frequency narrow range 2810 may be utilized in steps 2710 and 2720 of the method, minimum |S11| peak narrow range 2820 may be utilized in steps 2730 and 2740 of the method, and minimum |S11| peak total range 2840 may be utilized in steps 2750 and 2760 of the method. Thus, method 2700 may utilize the different frequency ranges to filter characteristics of an unknown material to identify the unknown material, such as to classify an unknown liquid as DI, alcohol, or vodka. For example, the various frequency ranges illustrated in FIG. 28 demonstrate that different liquids consistently exhibit certain properties when interrogated in accordance with embodiments of the present disclosure. This indicates that embodiments of the present disclosure are operable to identify liquids with a high degree of accuracy.

25 **[0096]** Referring to FIGs. 29-31, various aspects of a graphical user interface (GUI) for configuring a system for interrogation of a sample of an unknown material are shown. FIG. 29 illustrates an exemplary operations interface that may be utilized to execute the interrogation of a sample and compare signatures of the sample to one or more signatures in an existing database, such as the database 140 of FIG. 1. FIG 30 illustrates an exemplary interface for configuring various parameters, such as the frequency ranges, S-parameters, port impedance, and sampling data points, for interrogating a sample. The exemplary interface illustrated in FIG. 30 also facilitates configuration of a desired Smith chart format. FIG 31 illustrates various aspects of the exemplary interface illustrated in FIG. 30, and includes labels that identify the different functions provided by the exemplary interface. In FIGs. 32

and 33, diagrams illustrating various functional relationships of software modules that may be implemented in an interrogation system configured according to embodiments to provide the GUIs illustrated with reference to FIGs. 29-31 are shown. In some embodiments, the software modules may be stored as an application and/or instructions in a memory, such as memory 134 of FIG. 1. Fig. 30 is a flow diagram illustrating an exemplary method for identifying an unknown liquid according to an embodiment of the present disclosure.

[0097] Testing has shown that an interrogation system according to embodiments of the present disclosure is operable to noninvasively recognize or identify milk, milk mixed with water, milk mixed with alcohol, water, DI water, alcohol, liquor, coffee, carbonated drinks, such as sodas, and the like. Blind testing was also performed and resulted in accurate identification of one or more of these liquids. Additionally, testing has demonstrated that an interrogation system according to embodiments of the present disclosure is operable to recognize chemical reactions of two or more solutions within a container undergoing interrogation by an interrogation device according to embodiments of the present disclosure. For example, the signatures of the individual original solutions may be different from the solution that results after they are mixed together. Once the chemical reactions have completed, the changes in the S-parameters and/or in the Smith Chart become stable and the temporal variations can be used to identify the completion of chemical reactions. The similar principle is applied for detection of temperature changes in a liquid. For example, the signatures in the s-parameters and/or Smith Chart are different between water and ice. Thus, the temporal variations of the measurement can be used to identify the temperature changes in a solution. Further, monitoring has demonstrated that an interrogation system according to embodiments of the present disclosure is operable to test soil conditions, test solid particles in a solution, identify whole blood and plasma, test lubricants and oil, and the like, as explained above. For example, testing of soils conditions has been demonstrated by placing coils directly in samples of different soils and connected the coils to an electronic device (e.g., to form an interrogation system similar to the system 100 of FIG. 1). When water was applied to the soils, the signatures in the S-parameter and Smith Chart changed to indicate the moisture content of the soil samples. Additionally, analysis of whole blood and plasma with different viscosity and biochemical contents, such as glucose and iron, results in different signatures, thereby allowing conditions of blood or plasma to be identified by embodiments of the present disclosure. Further, signatures for lubricants and oils with various moisture contents and impurity particles may also be used to monitor the quality of the lubricant/oil in order to determine if they should be replaced (e.g., to protect mechanical components that utilize the

lubricant/oil). The embodiments of the present disclosure enable such applications to be performed continuously in situ, thus, providing a real-time monitoring system. Embodiments of an interrogation system according to the present disclosure may further be constructed to receive a finger and detect pulses, pulse rates and/or blood chemistry. For example, as blood
5 travels through the blood vessels and veins in the finger, changes in signatures generated by an interrogation system of embodiments configured to interrogate a finger may be observed and may be used to determine the pulse. In some embodiments, interrogation systems may be formed on flexible substrates that may be deformed to wrap around a cylinder or body part, such as a finger, or may be formed as a solid object, such as a ring, that may be worn to
10 provide real-time pulse monitoring. Additionally, some embodiments of the present interrogation systems may be extended to frequency ranges in microwaves or millimeter waves for miniature containers (e.g., micro or nano-droplets).

EXAMPLES

[0098] The present invention will be described in greater detail by way of specific
15 examples. The following examples are offered for illustrative purposes only and are not intended to limit the invention in any manner. Those of skill in the art will readily recognize a variety of noncritical parameters that can be changed or modified to yield essentially the same results.

[0099] An interrogator 100, having one coil with 5 turns wrapped around the body 116
20 was used to calculate the moisture content of three different soil samples: ASTM fine graded soil 3200, top soil 3210, and potting soil 3220. A commercial TDR sensor was also used to calculate the moisture content of the soils. The results for each sensor were generated and then compared. The sensors calculated the moisture content of each soil for five target moisture concentrations. The soil was dried in an oven to eliminate water content and then
25 prepared by mixing water to the soil based on the weight ratio of the target water content. The mixed soil was then loaded into a compaction mold 3230 and compressed using a soil compaction hammer 3240. For the TDR soil calculations, data was recorded four times at the same soil location using Insitu MRP Test software. For the interrogator soil calculations, data was recorded ten times at the same soil location using VNA. After the calculations were
30 made by the sensors, the water content of the soil was then measured again using dry density measurement to verify the target moisture concentration. The process was repeated for each soil at the five different target moisture concentrations.

SOIL 1: ASTM FINE GRADED (50-70) SAND

[0100] ASTM fine graded (50-70) sand was used to generate the test results at five target moisture concentrations: 2%, 5%, 8%, 11%, and 14%. The results of the moisture content calculations for the interrogator and TDR are shown below in Table 1. Taking the average for all five target concentrations, the interrogator results have approximately a twelve percent error when calculating the target water percentages. The TDR results are less accurate having, on average, approximately forty one percent error when calculating the target water percentages. The more accurate results of the interrogator are at least in part due to the frequency verification values. The frequency shift of the first, second and third feature verification can indicate the water percentages in the soil. The feature verification values can be used as parameters or signatures to verify the moisture content as described above.

Table 1: Results of ASTM Soil Calculations

Soil	Target Water Percentage	Interrogator Results (%)	TDR Results (%)	Feature Verification 1	Feature Verification 2	Feature Verification 3
ASTM soil	2	1.87	4.9	334.5	484.65	665.39
ASTM soil	5	4.48	6.46	301.95	441.6	593.5
ASTM soil	8	6.97	7.97	261.7	386.65	513.28
ASTM soil	11	8.81	9.94	250.5	370.2	494.1
ASTM soil	14	12.54	10.73	226	333.8	440.9

SOIL 2: TOP SOIL

[0101] Top Soil was used to generate the test results at five target moisture concentrations: 2%, 7%, 12%, 17%, and 22%. The results of the moisture content calculations for the interrogator and TDR are shown below in Table 2. Taking the average for all five target concentrations, the interrogator results have approximately a fourteen percent error when calculating the target water percentages for top soil. The TDR results are less accurate having, on average, approximately forty three percent error when calculating the target water percentages. The results for the top soil are similar to those found to the ASTM soil; however, a soil containing other materials such as organic matter will cause the TDR results to become inaccurate.

Table 2: Results of Top Soil Calculations

Soil	Target Water Percentage	Interrogator Results (%)	TDR Results (%)	Feature Verification 1	Feature Verification 2	Feature Verification 3
Top Soil	2	2.61	5.71	342.2	510.8	693.2
Top Soil	7	7.93	7.39	314.6	473.42	638.96
Top Soil	12	13.41	12.36	302.6	451.34	608.6
Top Soil	17	18.44	15.2	291.1	429.7	580.48
Top Soil	22	23.44	24.75	257.99	381.4	508.8

SOIL 2: POTTING SOIL

[0102] Potting Soil was used to generate the test results at five target moisture concentrations: 2%, 7%, 12%, 17%, and 22%. The results of the moisture content calculations for the interrogator and TDR are shown below in Table 1. Potting soil contains a lot of different materials; some common ingredients used in potting soil are peat, composted bark, sand, perlite and recycled mushroom compost. Potting soil is also aerated making calculation of the moisture content difficult. As a result, the Interrogator results have, on average, approximately a forty five percent error when calculating the target water percentages for potting soil. The TDR results fair much worse having over one thousand percent error when calculating the water percentage in potting soil. The introduction of new materials and air have a less harmful effect of the interrogator results partly because the feature verification values can still be used to cross check the results of the interrogator, as described above.

Table 3: Results of Potting Soil Calculations

Soil	Target Water Percentage	Interrogator Results (%)	TDR Results (%)	Feature Verification 1	Feature Verification 2	Feature Verification 3
Potting soil	2	5.12	55.07	238.6	409.4	597.7
Potting soil	7	8.11	108.8	233.7	405.06	580.2
Potting soil	12	10	202.17	228.1	399.32	570.19
Potting soil	17	19.89	11.85	214.1	374.19	536.1
Potting soil	22	26.75	9.81	209.27	361.38	532.8

* * *

[0103] The above specification and examples provide a complete description of the structure and use of illustrative embodiments. Although certain embodiments have been described above with a certain degree of particularity, or with reference to one or more individual embodiments, those skilled in the art could make numerous alterations to the disclosed embodiments without departing from the scope of this invention. As such, the various illustrative embodiments of the methods and systems are not intended to be limited to the particular forms disclosed. Rather, they include all modifications and alternatives falling within the scope of the claims, and embodiments other than the one shown may include some or all of the features of the depicted embodiment. For example, elements may be omitted or combined as a unitary structure, and/or connections may be substituted. Further, where appropriate, aspects of any of the examples described above may be combined with aspects of any of the other examples described to form further examples having comparable or different properties and/or functions, and addressing the same or different problems. Similarly, it will be understood that the benefits and advantages described above may relate to one embodiment or may relate to several embodiments.

[0104] The claims are not intended to include, and should not be interpreted to include, means-plus- or step-plus-function limitations, unless such a limitation is explicitly recited in a given claim using the phrase(s) “means for” or “step for,” respectively.

CLAIMS

1. A method for determining one or more characteristics of a material, the method comprising:
 - exciting one or more conductive coils with a source signal, where the one or more conductive coils surround a volume;
 - monitoring one or more parameters associated with each of the one or more conductive coils during the exciting;
 - determining one or more signatures associated with a material within the volume based on the one or more parameters; and
 - comparing the one or more signatures to one or more candidate signatures to identify the material.
2. The method of claim 1, where the one or more parameters associated with each of the one or more conductive coils comprise: one or more scattering parameters, a resonance frequency, a shape and location of curves in a Smith Chart, or a combination thereof.
3. The method of claim 2, further comprising varying a frequency of the source signal at which at least one of the one or more coils is excited.
4. The method of any of claims 2-3, where the one or more candidate signatures correspond to signatures representative of at least one known material, and where the signatures representative of the at least one known material are determined based one or more parameters determined while the at least one known materials was disposed within the volume.
5. The method of claim 4, where comparing the one or more signatures to the one or more candidate signatures comprises comparing, at each of a set of frequencies, a determined parameter corresponding to the material with a corresponding known parameter corresponding to the at least one known material.
6. The method of claim 5, where comparing, at each of the set of frequencies, the determined parameter with the corresponding known parameter comprises comparing a Smith chart of the determined parameter with a Smith chart of the corresponding known parameter.

7. The method of any of claims 1-6, where the one or more coils comprise two or more coils.
8. The method of any of claims 1-7, where at least one of the one or more coils comprises two or more turns.
9. The method of any of claims 1-8, where at least one of the one or more coils comprises four or more turns.
10. The method of any of claims 1-9, where a maximum transverse dimension of the core volume is approximately 4 centimeters (cm) or larger.
11. The method of any of claims 1-10, where:
each of the one or more coils is coupled to a body that defines an interior channel
within the volume; and
the material is disposed within the interior channel.
12. The method of claim 11, where the material is disposed within a container that is disposed within the interior channel.
13. The method of claim 11 or 12, where the body is flexible.
14. The method of claim 11, where the body comprises a pipe through which the material flows.
15. The method of any of claims 1-14, where the material comprises water, alcohol, coffee, a soft drink, milk, oil, blood, or a combination thereof.
16. The method of any of claims 1-15, where the one or more characteristics of the material includes an alcohol content of the material.
17. The method of any of claims 1-16, where:
the material comprises soil; and
the one or more characteristics of the material includes a moisture content of the soil.

18. The method of any of claims 1-16, where:
 - the material comprises a liquid and a solid; and
 - the one or more characteristics of the material includes a solids content of the material.
19. The method of any of claims 1-16, where:
 - the material comprises blood; and
 - the one or more characteristics of the material includes a plasma content of the blood.
20. The method of any of claims 1-19, where the one or more characteristics of the material includes a temperature of the material.
21. A system for determining one or more characteristics of a material, the system comprising:
 - one or more conductive coils surrounding a volume;
 - one or more signal generators, each configured to be coupled to a respective one of the one or more coils and to excite the respective coil with a respective source signal;
 - one or more signal receivers, each configured to be coupled to a respective one of the one or more coils and to monitor one or more parameters associated with the respective conductive coil during the exciting; and
 - a processor configured to:
 - determine one or more signatures associated with a material within the volume based on the one or more parameters; and
 - compare the one or more signatures to one or more candidate signatures to identify the material.
22. The system of claim 21, where the one or more parameters associated with each of the one or more conductive coils comprise: one or more scattering parameters, a resonance frequency, a shape and location of curves in a Smith Chart, or a combination thereof.
23. The system of claim 22, where at least one of the one or more signal generators is configured to vary the frequency of the respective source signal at which the respective coil is excited.

24. The system of claim 23, where the frequency of the respective source signal used to excite the respective coil is between approximately 200 megahertz (MHz) and approximately 400 MHz.
25. The system of claim 23 or 24, where the processor is configured to determine a resonance frequency associated with at least one of the one or more coils at least by:
- determining, for each frequency of a set of frequencies at which the at least one coil is excited, a reflection coefficient, a transmission coefficient, and/or a scattering parameter that is associated with the at least one coil; and
 - identifying, as the resonance frequency, the frequency of the set of frequencies at which the magnitude of the reflection coefficient and/or the magnitude of the scattering parameter is smallest and/or at which the magnitude of the transmission coefficient is largest.
26. The system of any of claims 22-25, where the one or more candidate signatures correspond to signatures representative of at least one known material, and where the signatures representative of the at least one known material are determined based one or more parameters determined while the at least one known materials was disposed within the volume.
27. The system of claim 26, where the processor is configured to compare the one or more determined parameters with the one or more corresponding known parameters at least by comparing, at each of a set of frequencies, a determined parameter corresponding to the material with a corresponding known parameter corresponding to the at least one known material.
28. The system of claim 27, where the processor is configured to compare, at each of the set of frequencies, the determined parameter with the corresponding known parameter at least by comparing a Smith chart of the determined parameter with a Smith chart of the corresponding known parameter.
29. The system of any of claims 21-28, where the one or more coils comprises two or more coils.
30. The system of any of claims 21-29, where at least one of the one or more coils comprises two or more turns.

31. The system of any of claims 21-30, where at least one of the one or more coils comprises four or more turns.
32. The system of any of claims 21-31, where a maximum transverse dimension of the core volume is approximately 4 cm or larger.
33. The system of any of claims 21-32, where each of the one or more coils is coupled to a body that defines an interior channel within the core volume, the interior channel configured to receive the material.
34. The system of claim 33, where the body is flexible.
35. The system of claim 33, where the body comprises a pipe configured to convey the material.
36. The system of any of claims 21-35, where the material comprises water, alcohol, coffee, a soft drink, milk, oil, blood, or a combination thereof.
37. The system of any of claims 21-36, where the one or more characteristics of the material includes an alcohol content of the material.
38. The system of any of claims 21-37, where:
the material comprises soil; and
the one or more characteristics of the material includes a moisture content of the soil.
39. The system of any of claims 21-37, where:
the material comprises a liquid and a solid; and
the one or more characteristics of the material includes a solids content of the material.
40. The system of any of claims 21-37, where:
the material comprises blood; and
the one or more characteristics of the material includes a plasma content of the blood.
41. The system of any of claims 21-40, where the one or more characteristics of the material includes a temperature of the material.

42. A non-transitory computer-readable storage medium storing instructions that, when executed by a processor, cause the processor to perform operations for determining one or more characteristics of a material, the operations comprising:

exciting one or more conductive coils with a source signal, where the one or more conductive coils surround a volume;
monitoring one or more parameters associated with each of the one or more conductive coils during the exciting;
determining one or more signatures associated with a material within the volume based on the one or more parameters; and
comparing the one or more signatures to one or more candidate signatures to identify the material.

43. The non-transitory computer-readable storage medium of claim 42, where the one or more parameters associated with each of the one or more conductive coils comprise: a reflection coefficient, a transmission coefficient, a scattering parameter, a resonance frequency, or a combination thereof.

44. The non-transitory computer-readable storage medium of claim 43, the operations further comprising varying a frequency of the source signal at which at least one of the one or more coils is excited.

45. The non-transitory computer-readable storage medium of claim 44, where the frequency of the source signal used to excite the coil is between approximately 200 megahertz (MHz) and approximately 400 MHz.

46. The method of claim 44 or 45, further comprising determining, during the monitoring, a resonance frequency associated with each of the one or more conductive coils at least by:

setting the frequency of the source signal at which each of the one or more conductive coils is excited to each of a set of frequencies;
determining, for each frequency of the set of frequencies, a reflection coefficient, a transmission coefficient, and/or a scattering parameter associated with each of the one or more conductive coils; and
identifying, as the resonance frequency, the frequency of the set of frequencies at which the magnitude of the reflection coefficient and/or the magnitude of the

scattering parameter is smallest and/or at which the magnitude of the transmission coefficient is largest.

47. The method of any of claims 43-46, where the one or more candidate signatures correspond to signatures representative of at least one known material, and where the signatures representative of the at least one known material are determined based one or more parameters determined while the at least one known materials was disposed within the volume.

48. The method of claim 47, where comparing the one or more signatures to one or more candidate signatures comprises comparing, at each of a set of frequencies, a determined parameter corresponding to the material with a corresponding known parameter corresponding to the at least one known material.

49. The method of claim 48, where comparing, at each of the set of frequencies, the determined parameter with the corresponding known parameter comprises comparing a Smith chart of the determined parameter with a Smith chart of the corresponding known parameter.

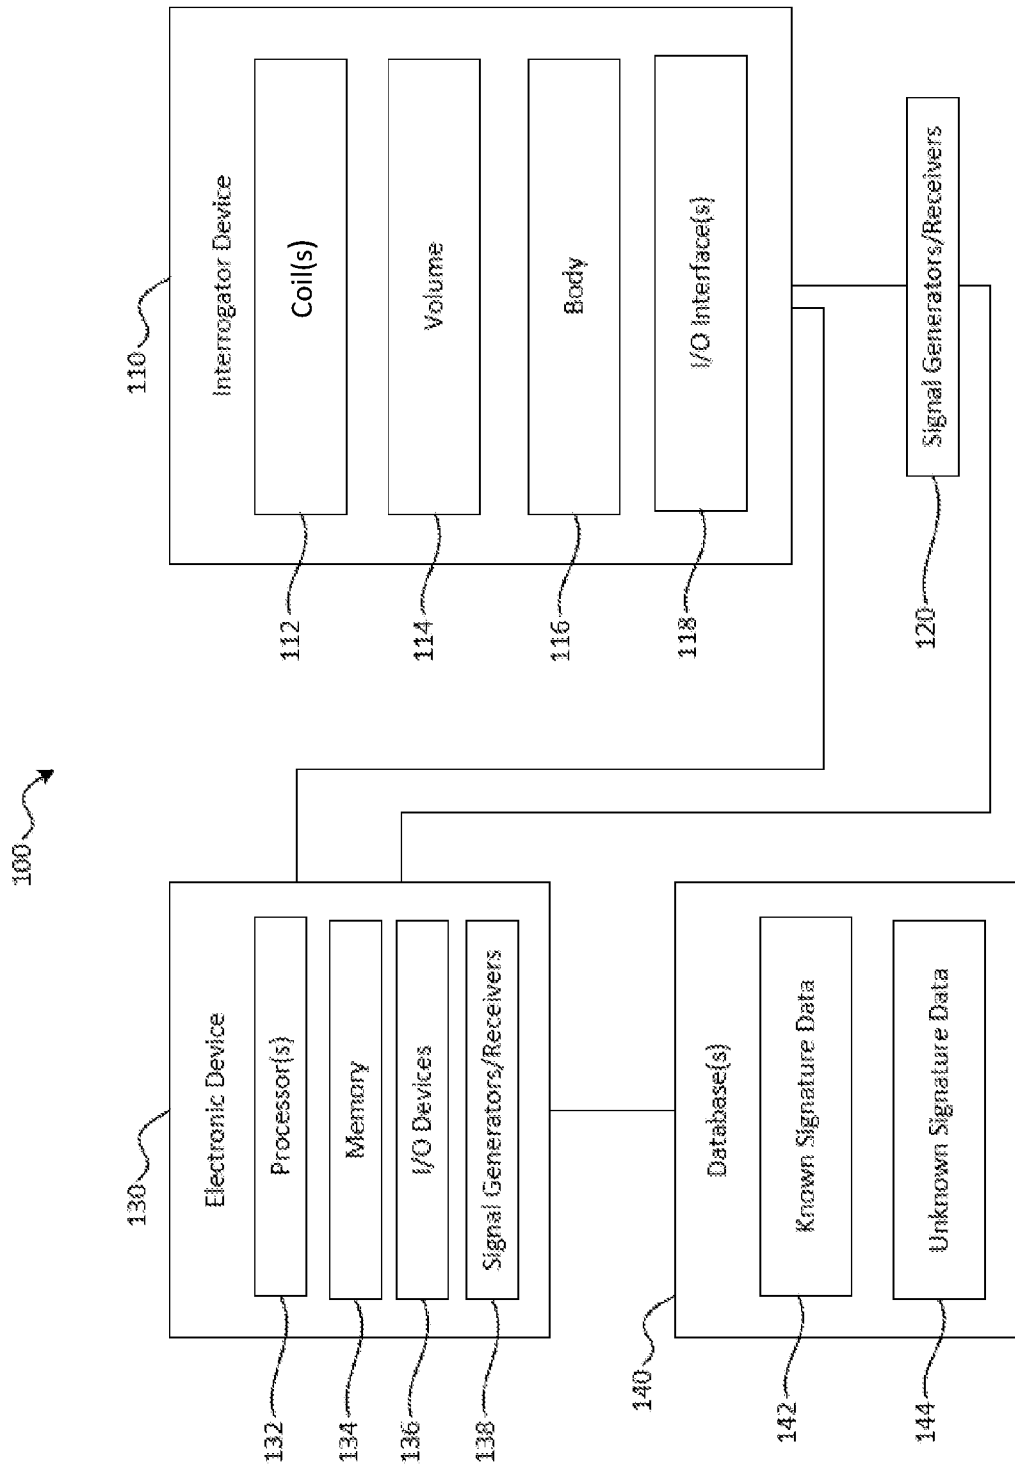


FIG. 1

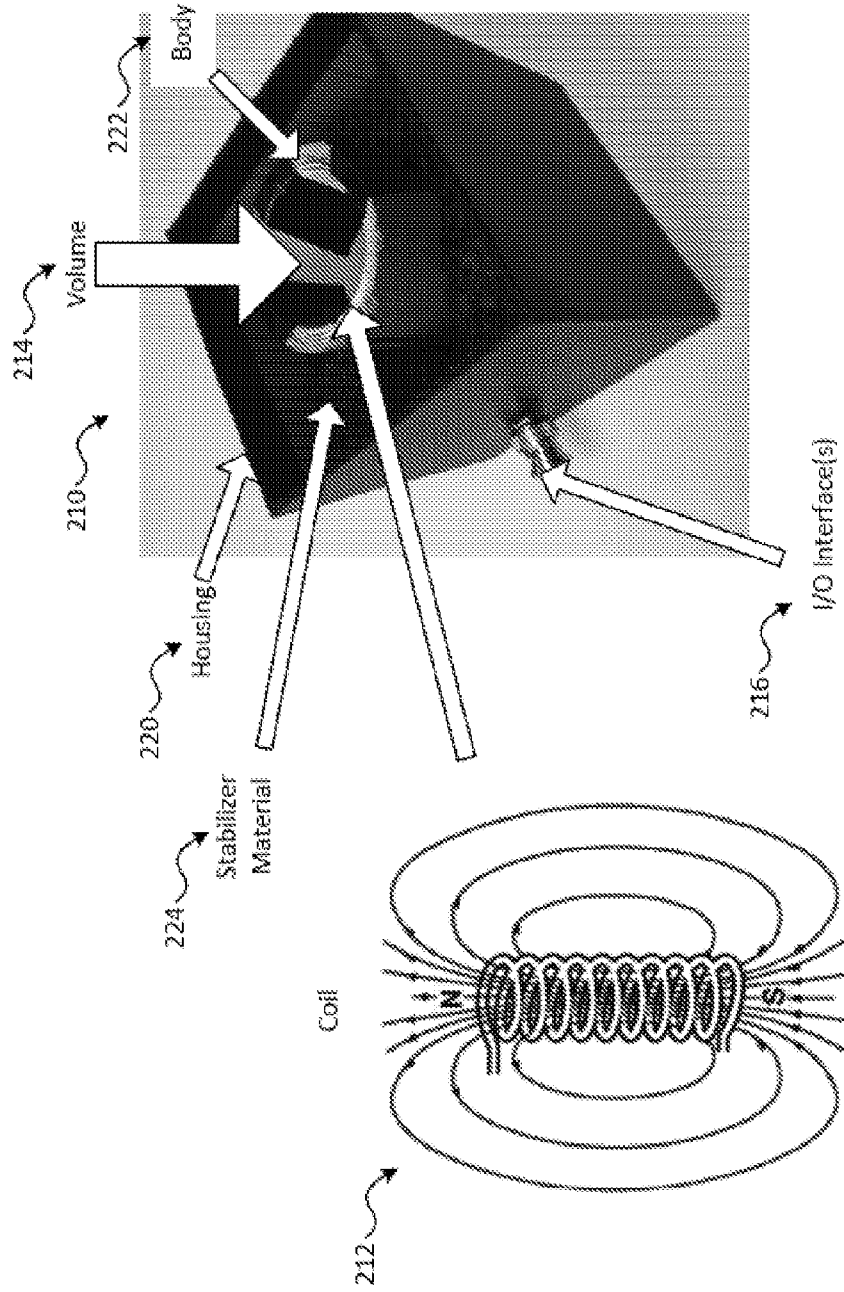


FIG. 2

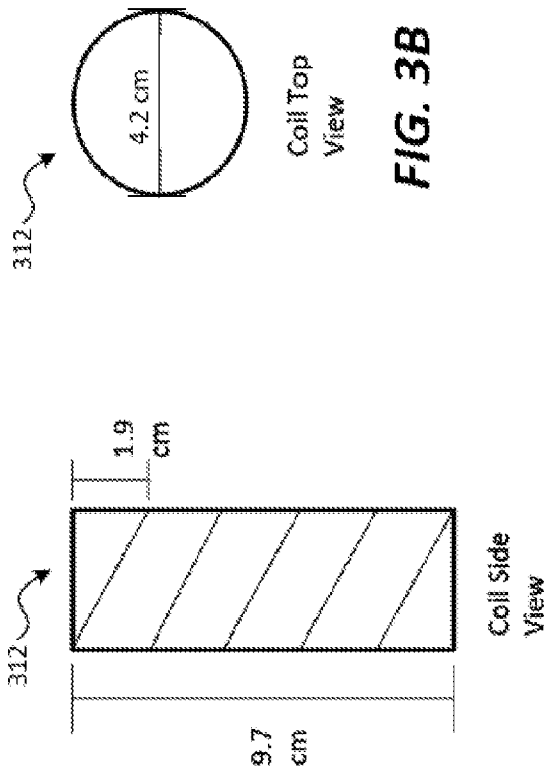


FIG. 3A

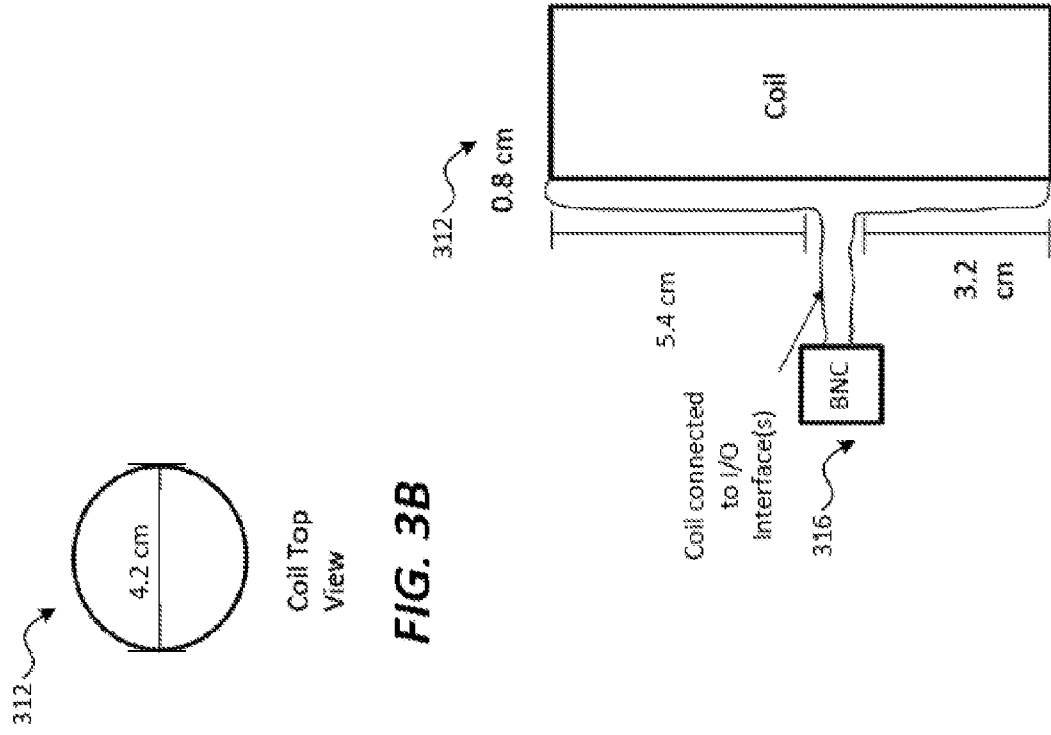


FIG. 3B

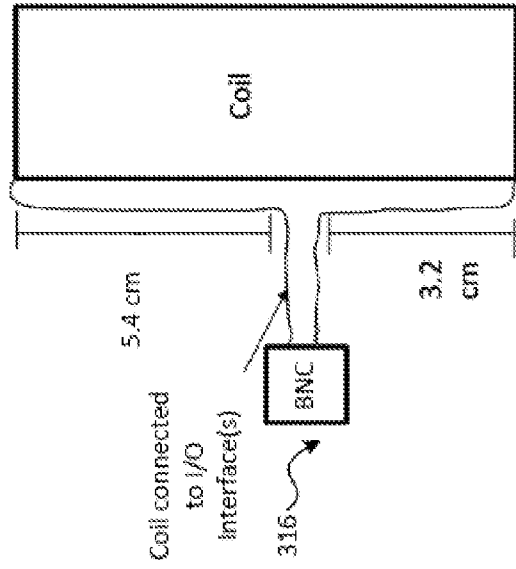


FIG. 3C

FIG. 3A

4/35

400

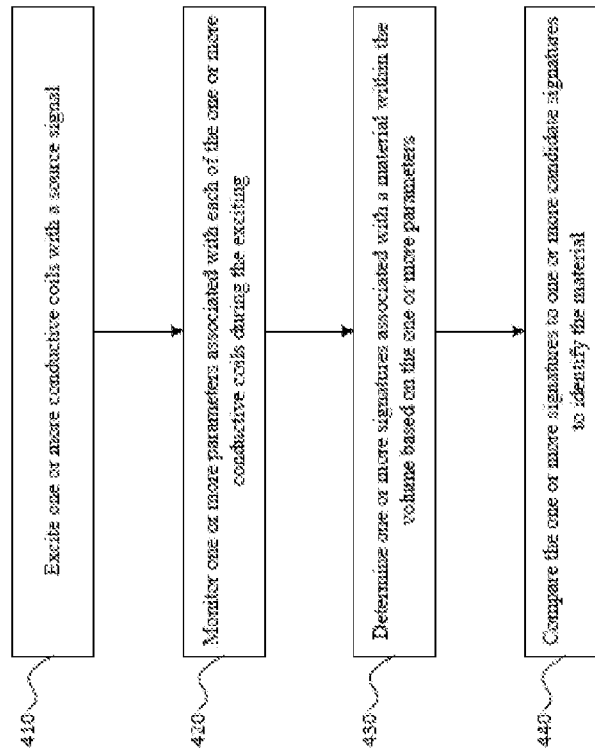


FIG. 4

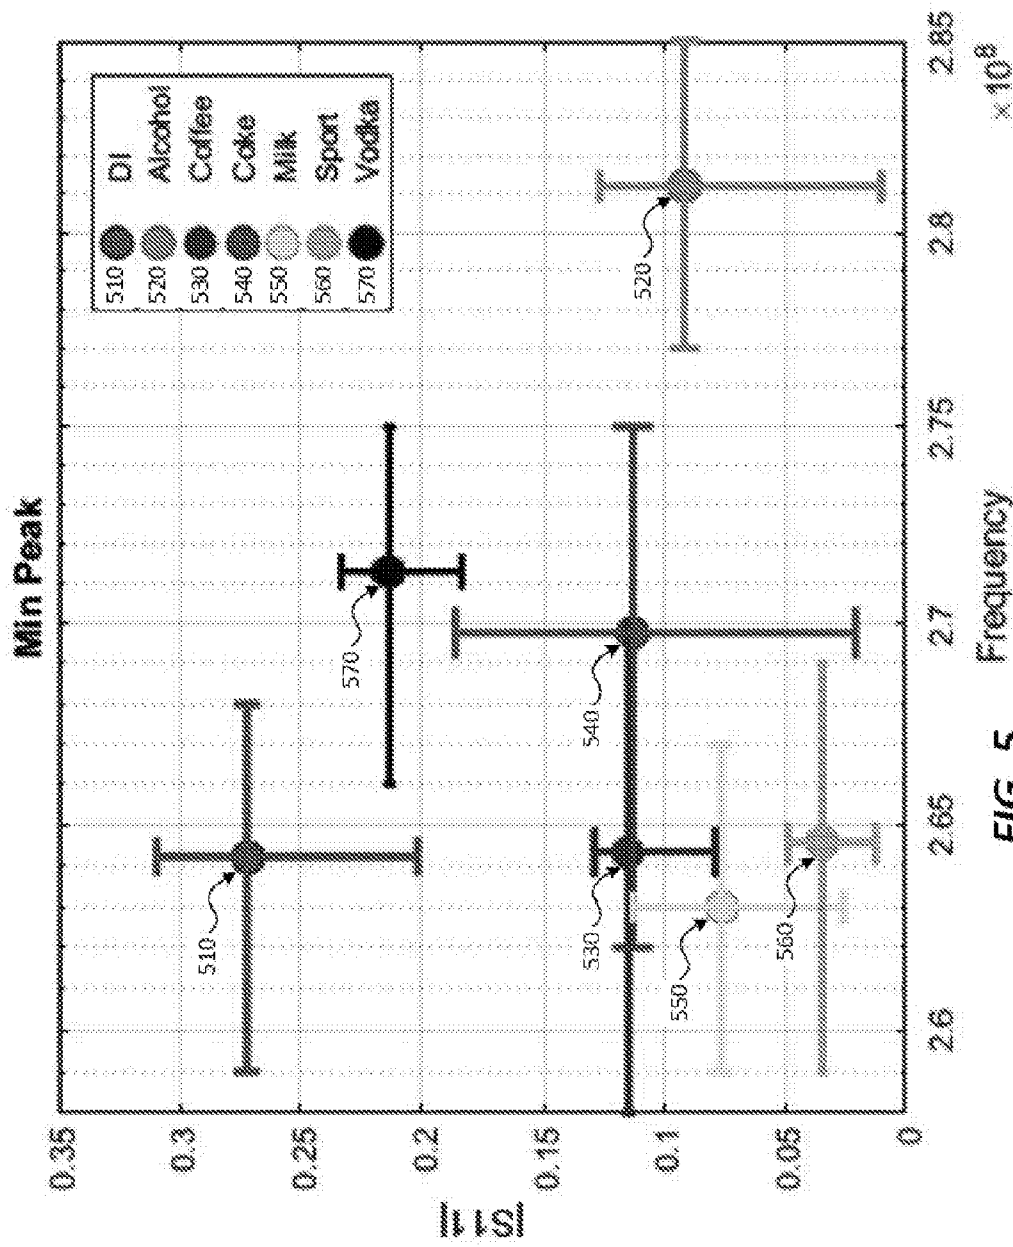


FIG. 5

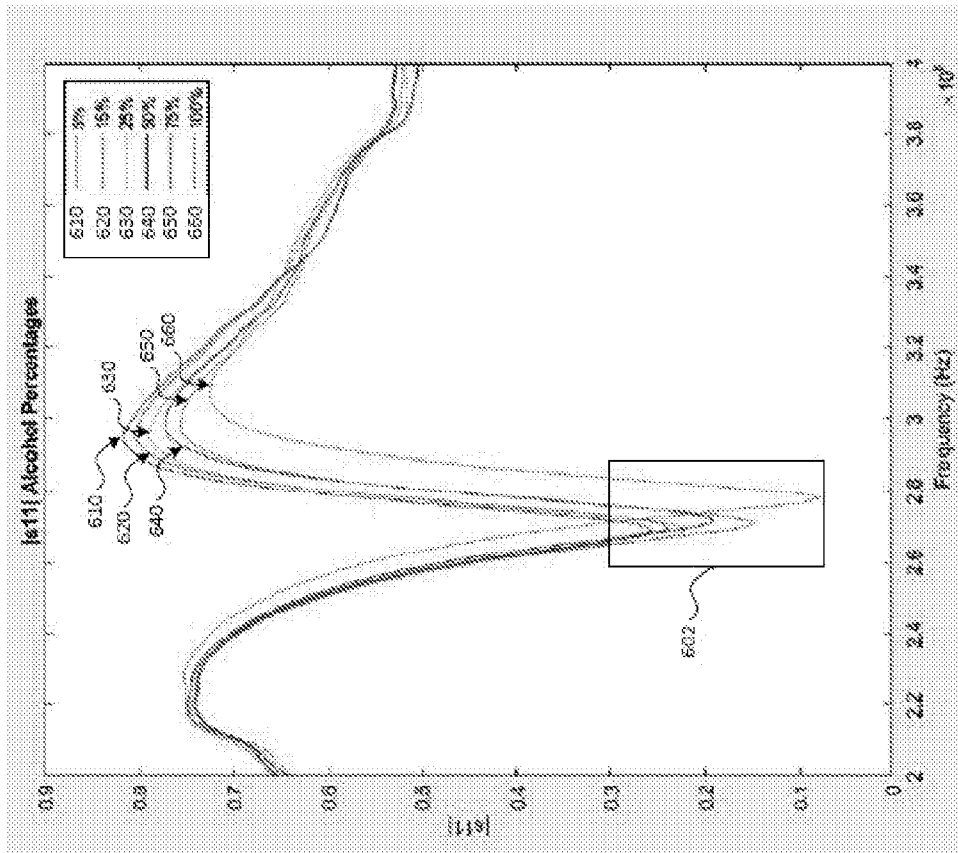


FIG. 6

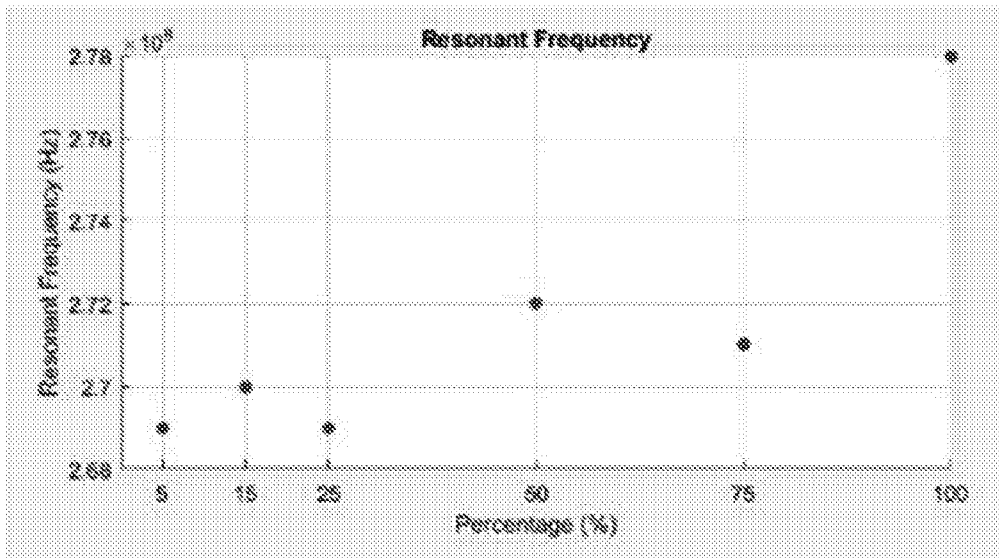


FIG. 7

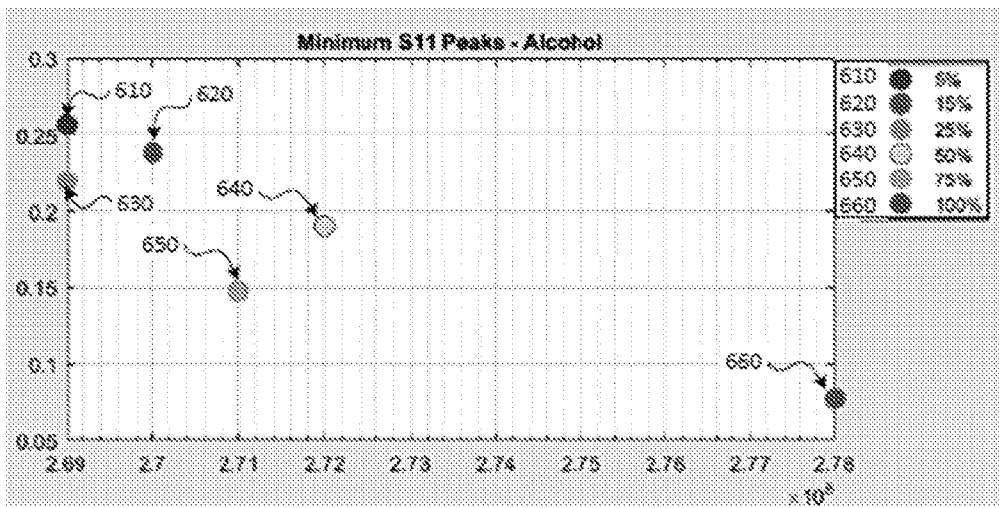
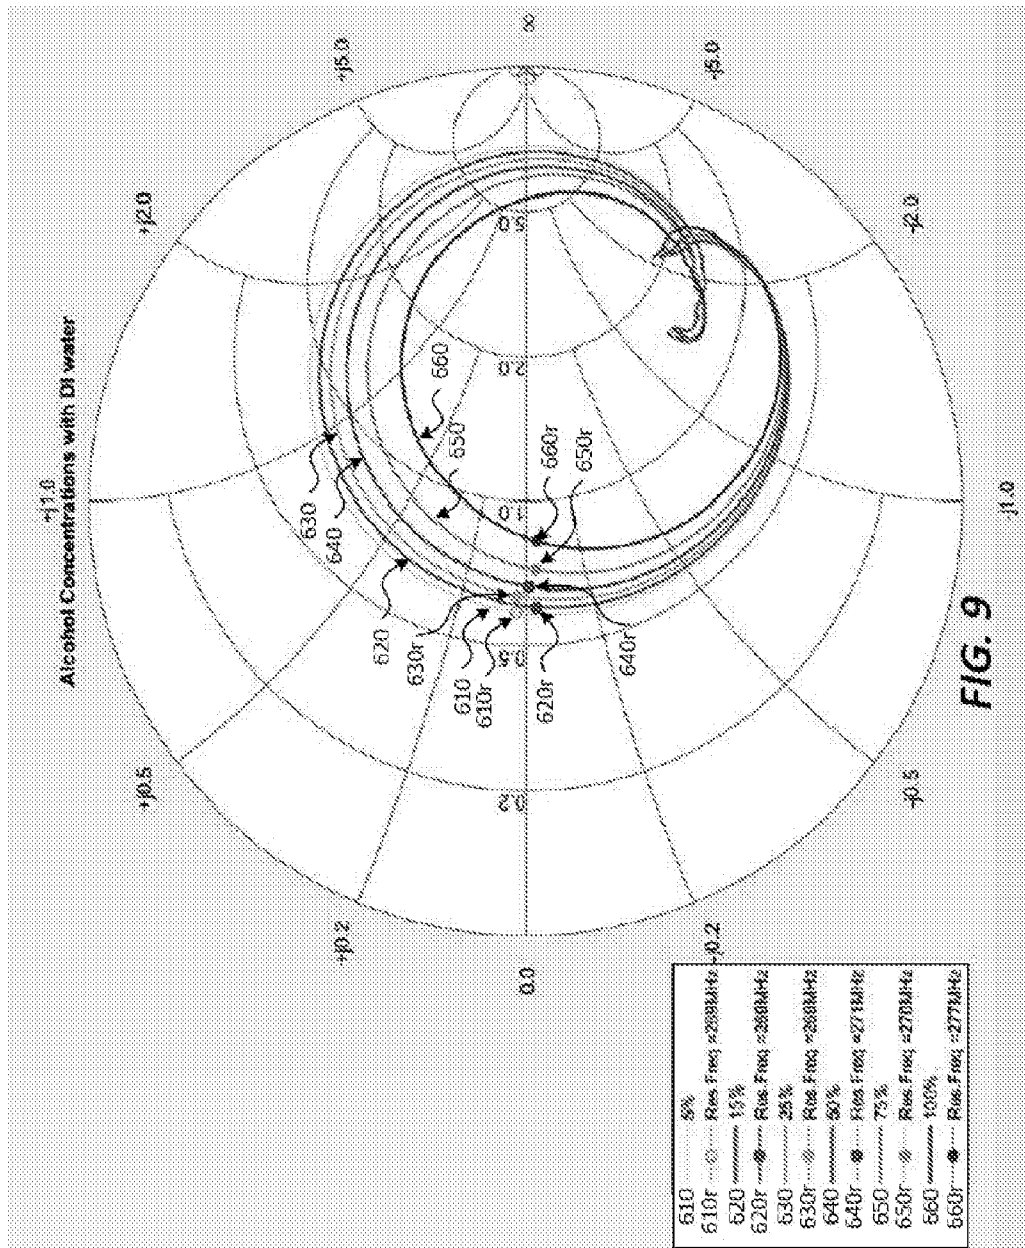


FIG. 8



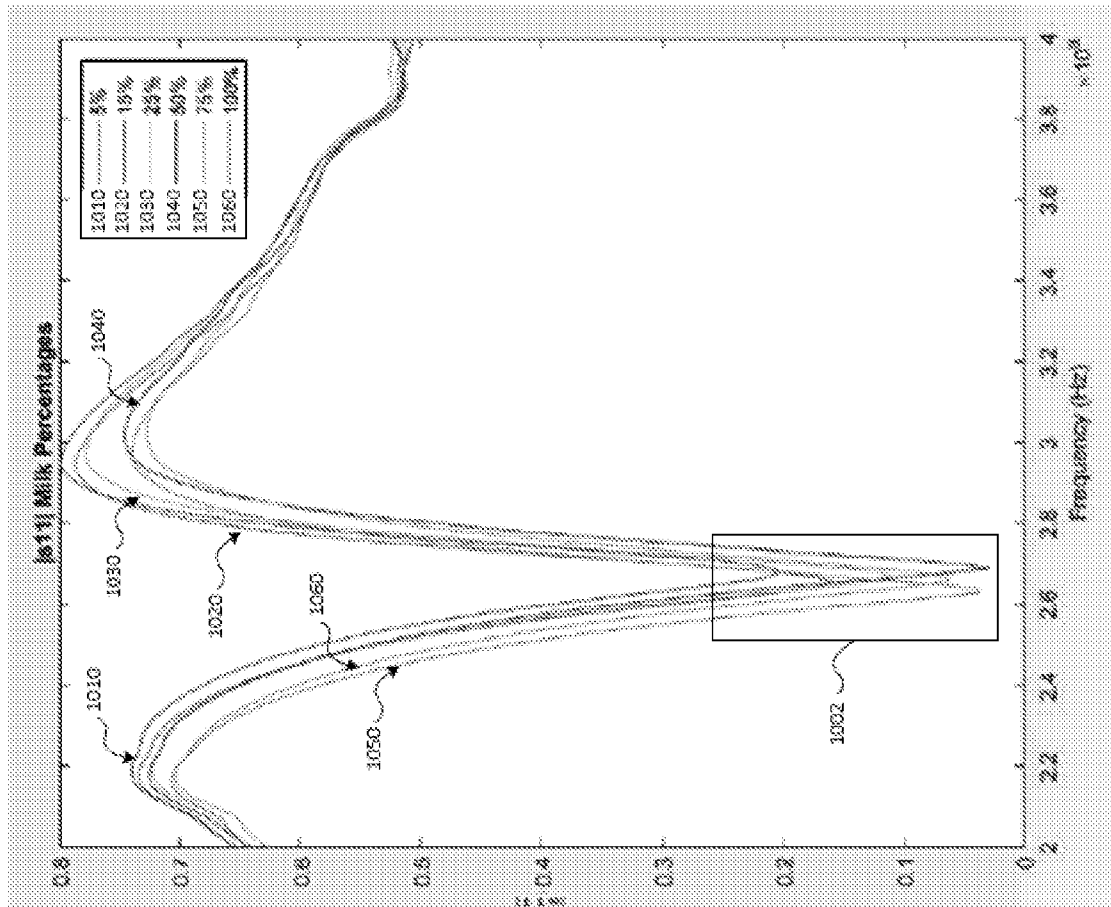


FIG. 10

10/31

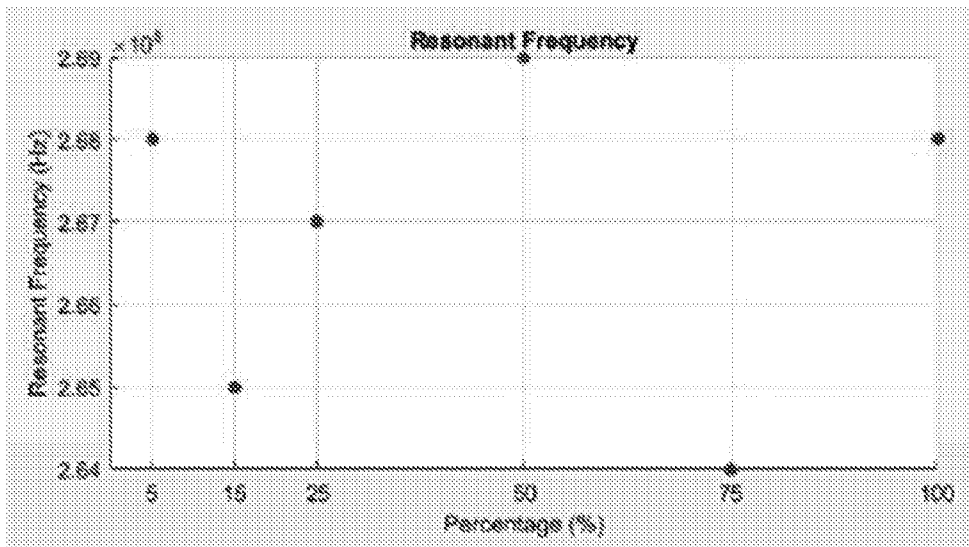


FIG. 11


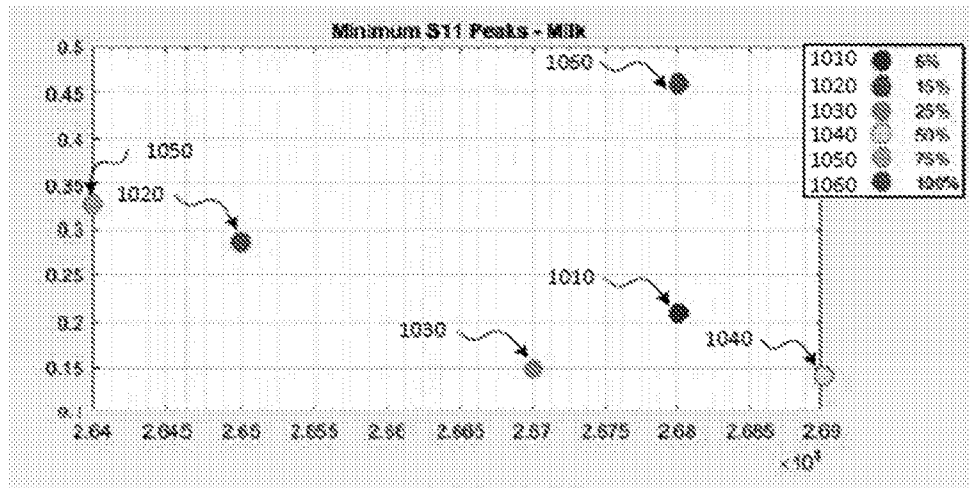


FIG. 12

11/31

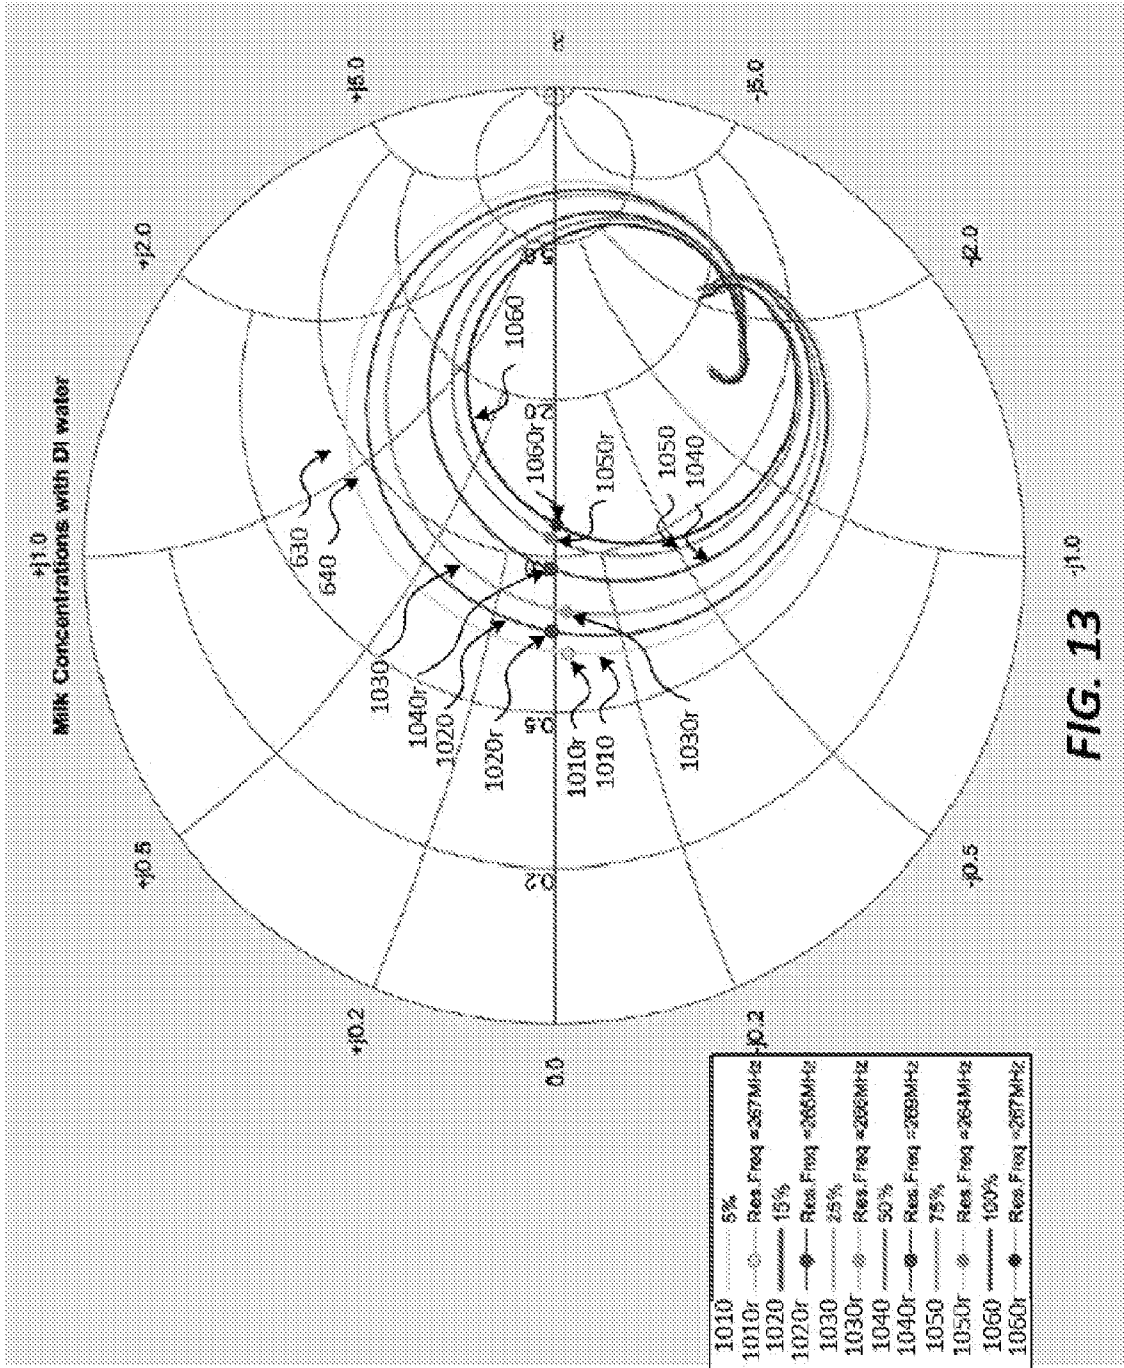

12/31

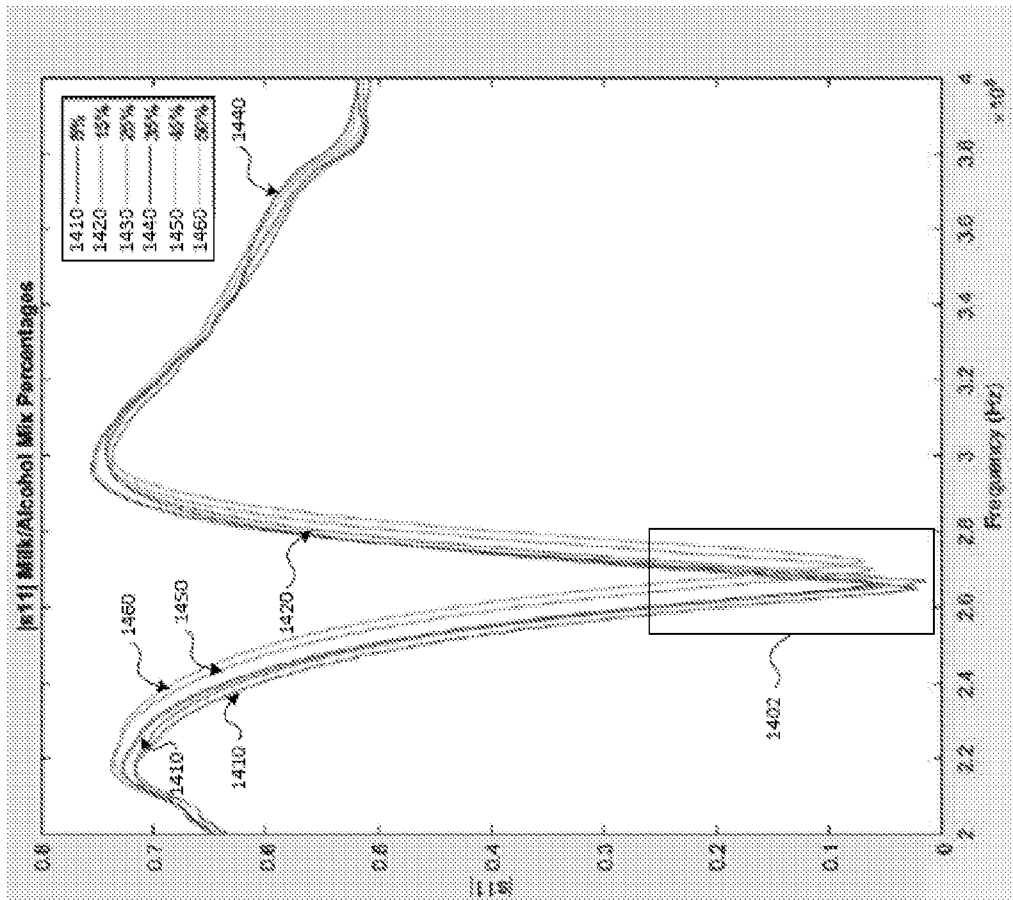


FIG. 14

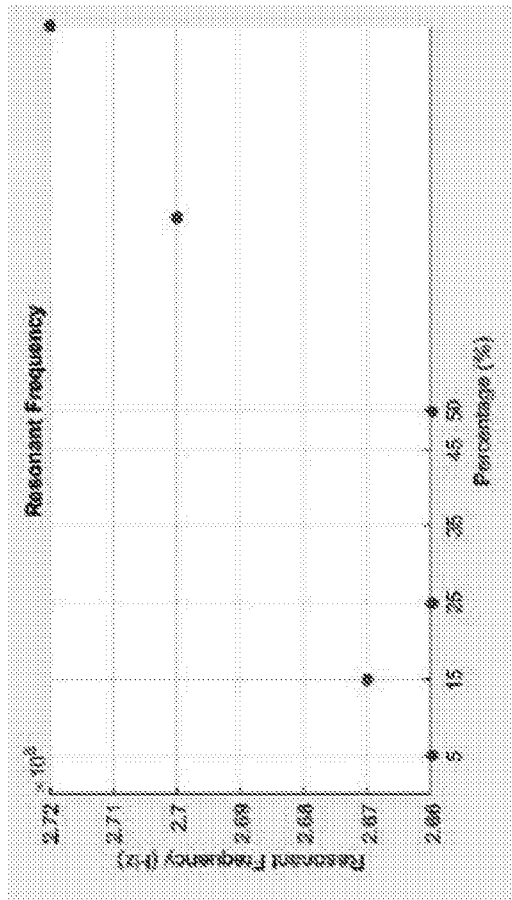


FIG. 15

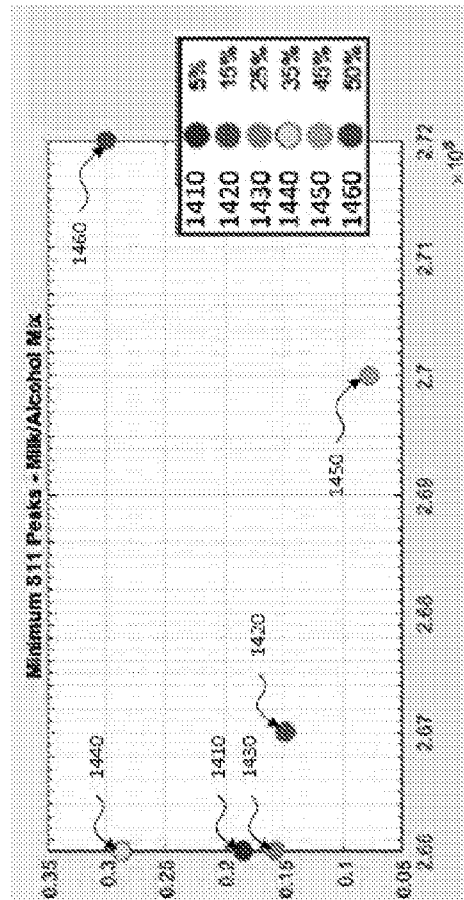


FIG. 16

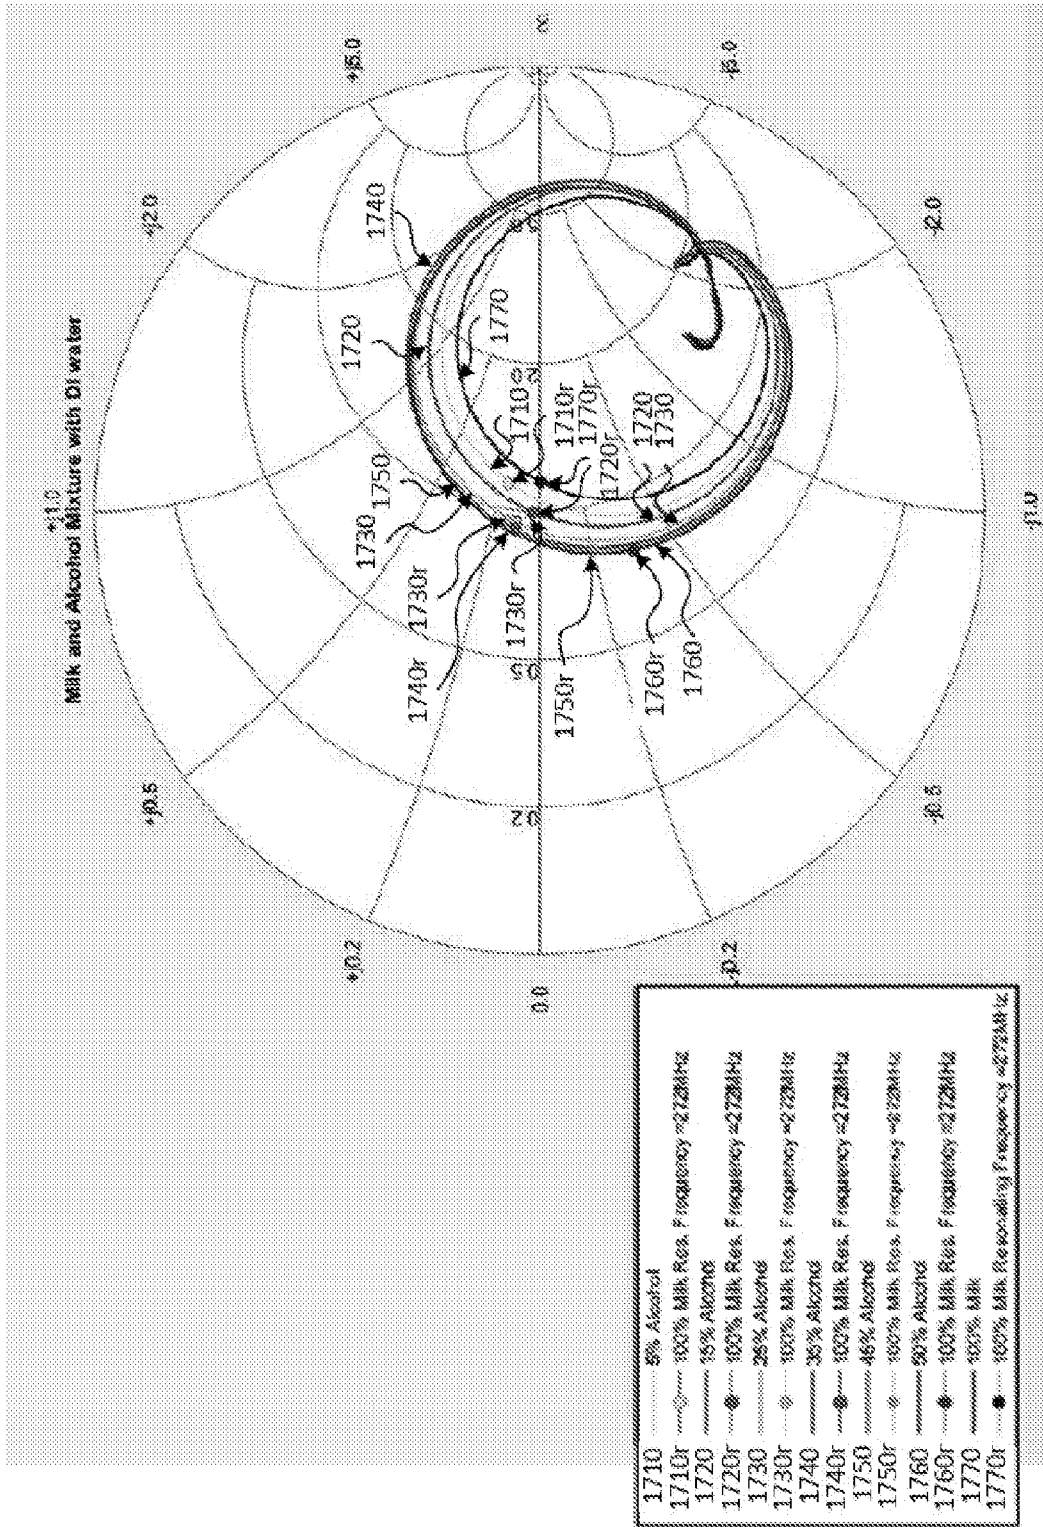


FIG. 17

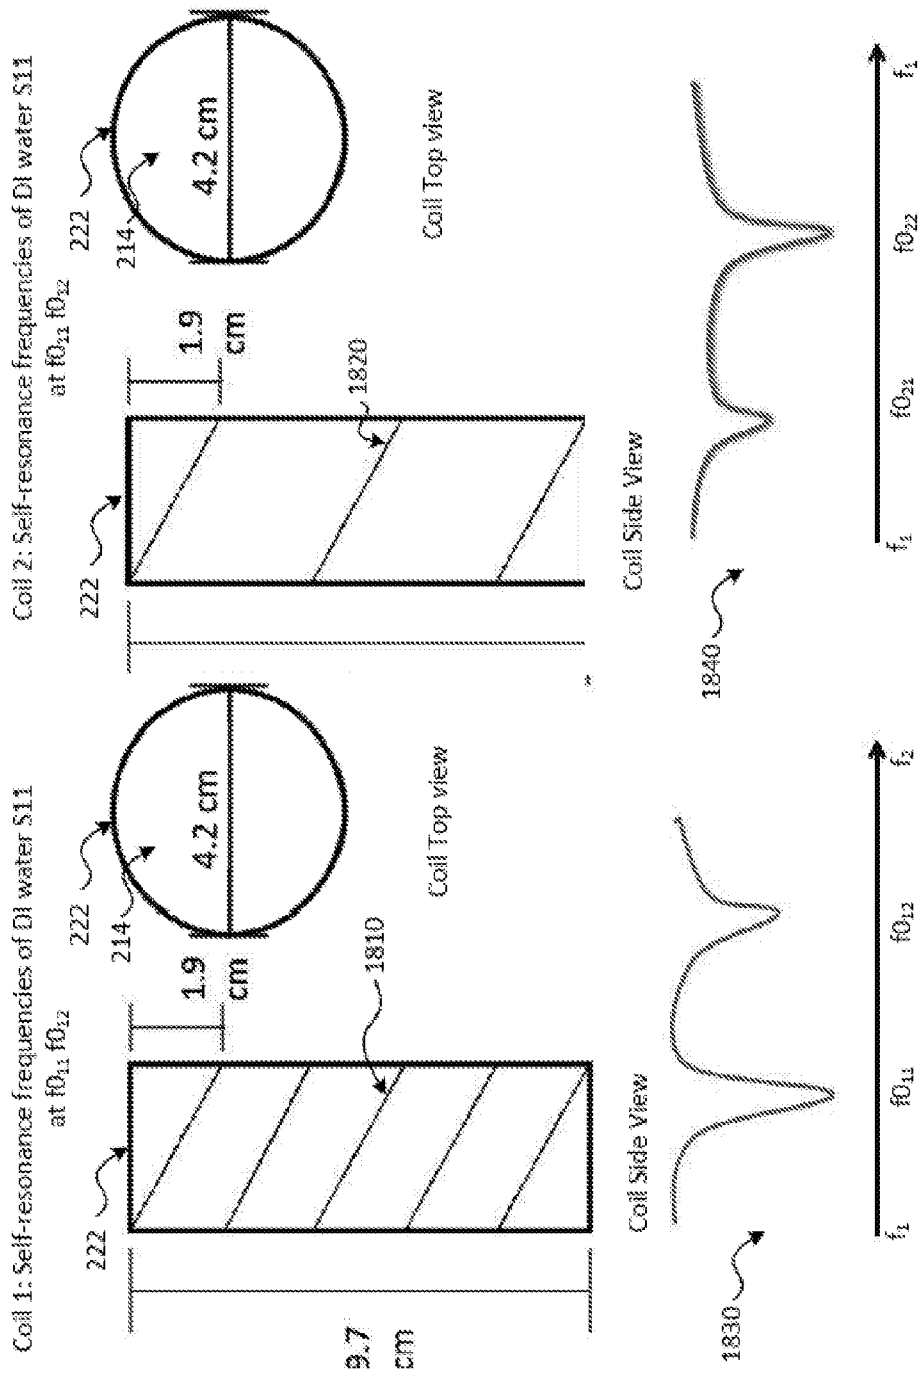


FIG. 18A

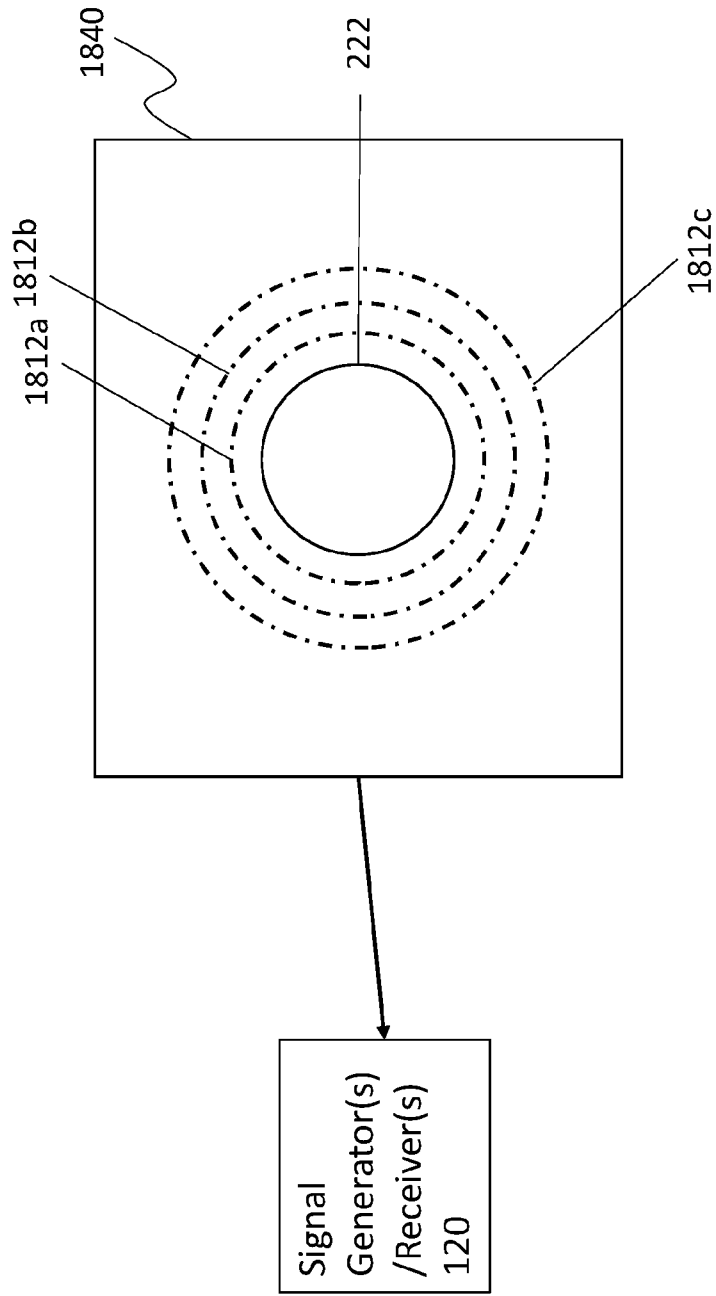


FIG. 18B

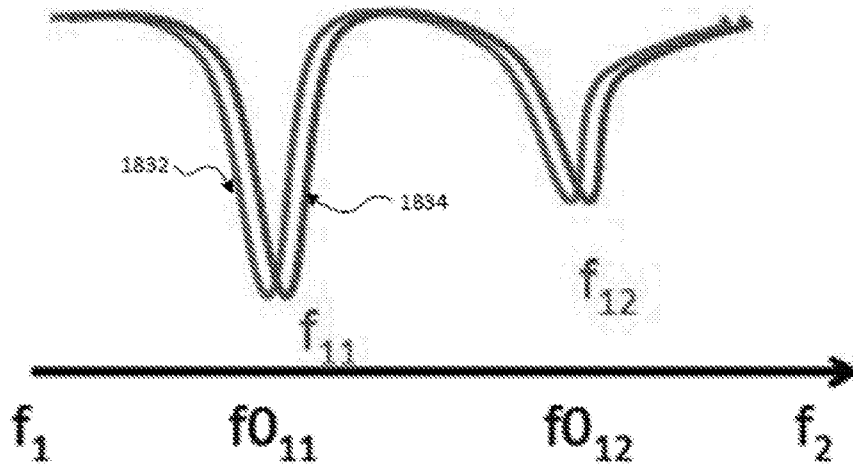


FIG. 19

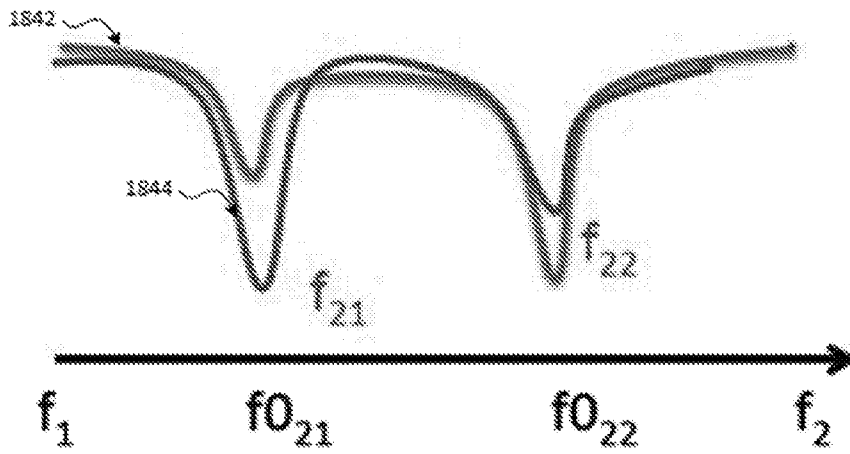


FIG. 20

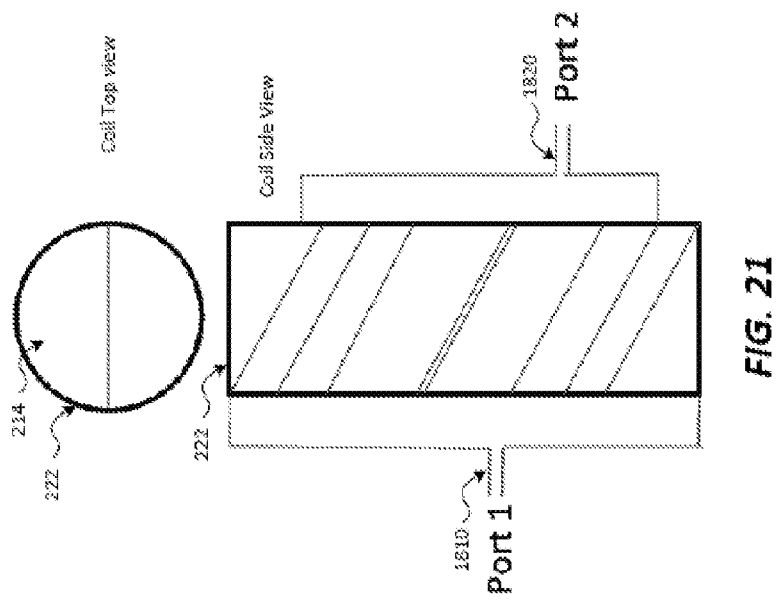


FIG. 21

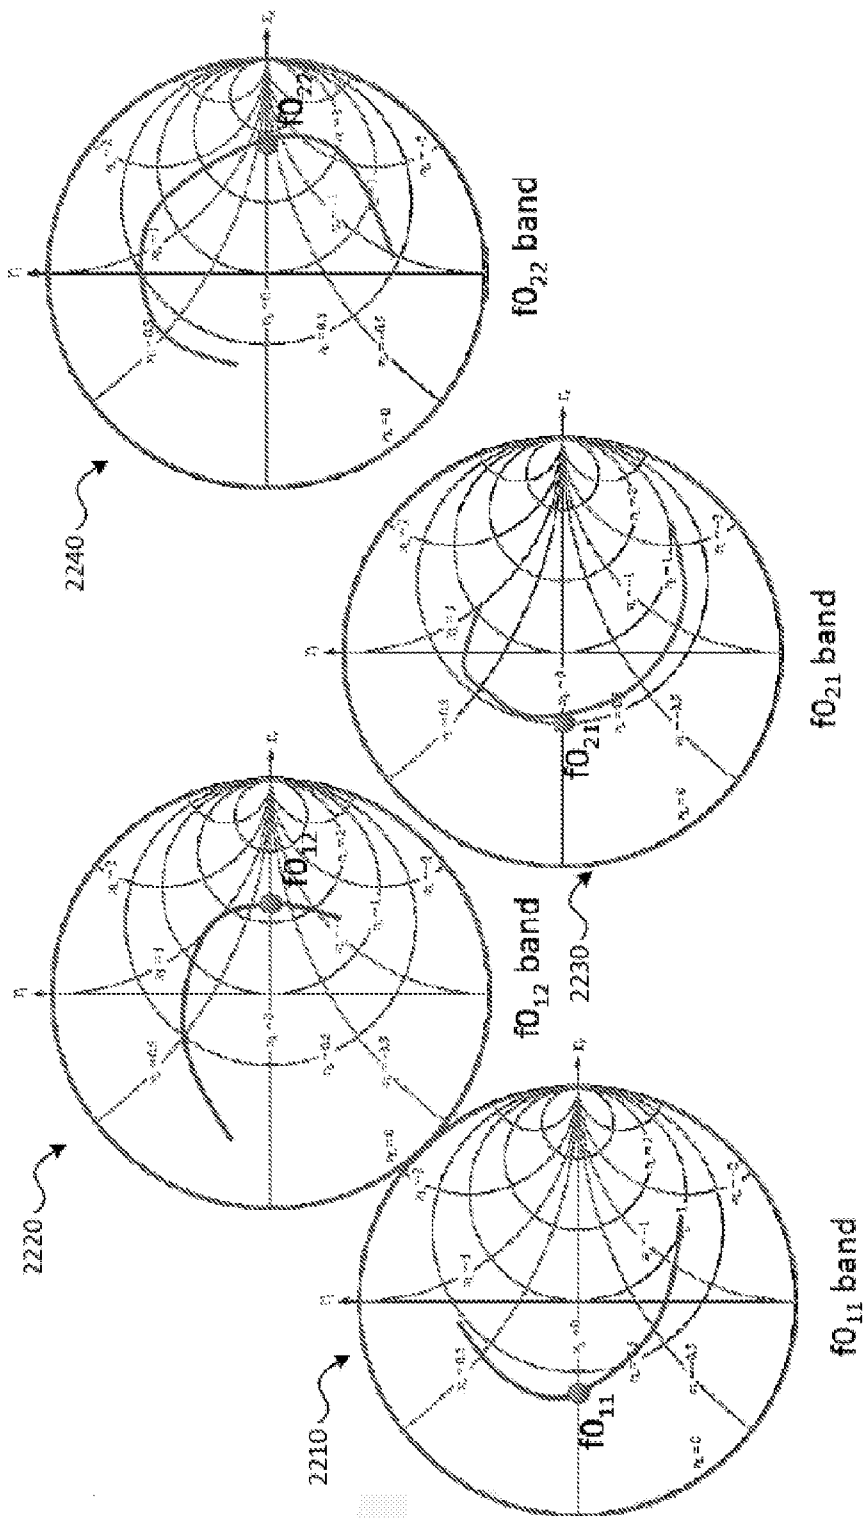


FIG. 22

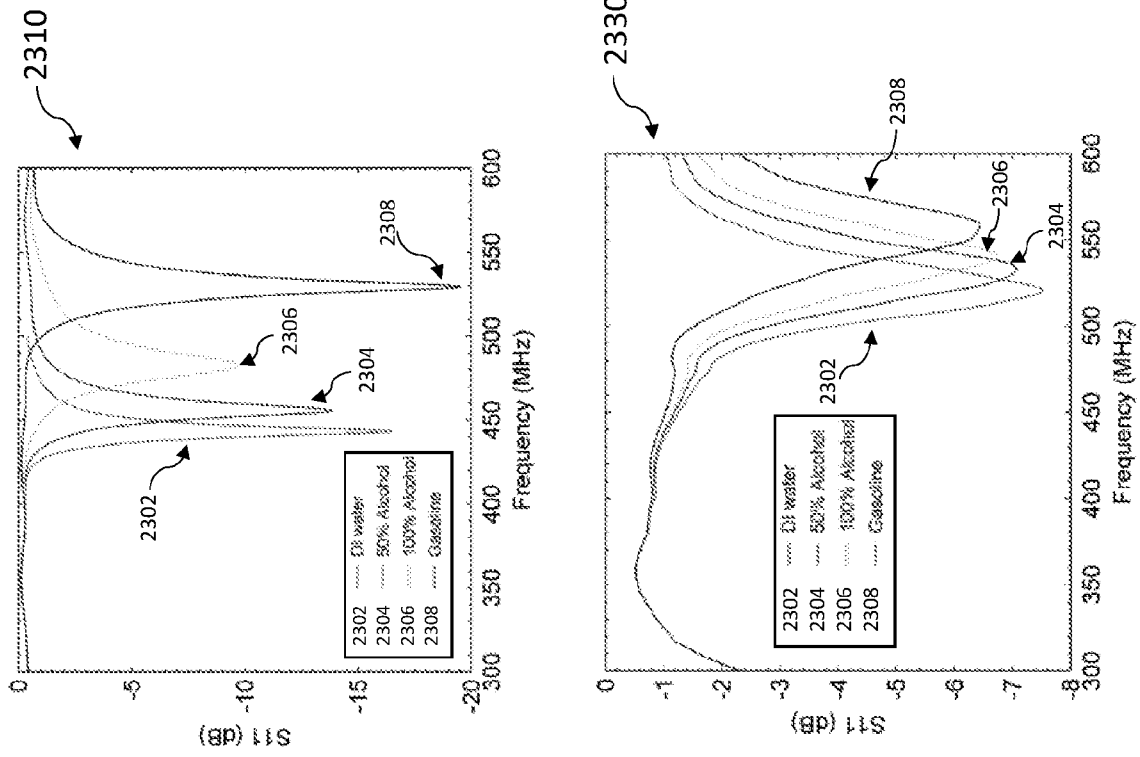
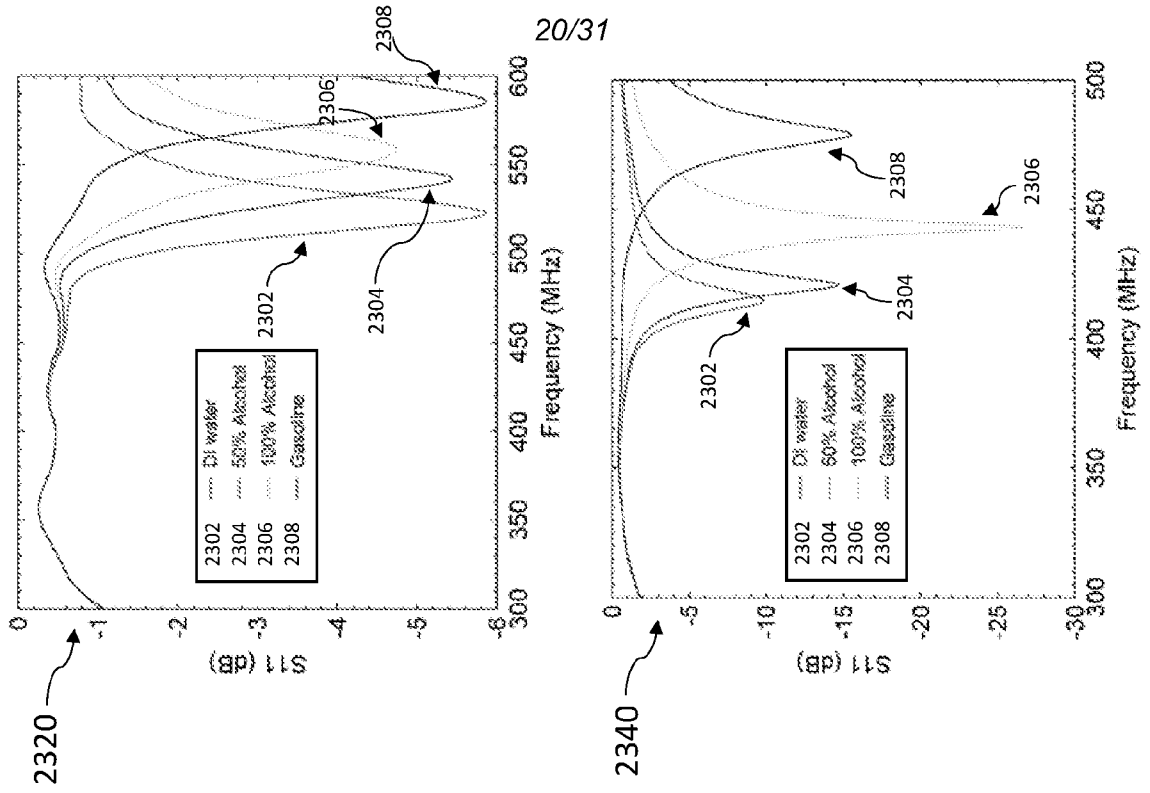


FIG. 23

21/31

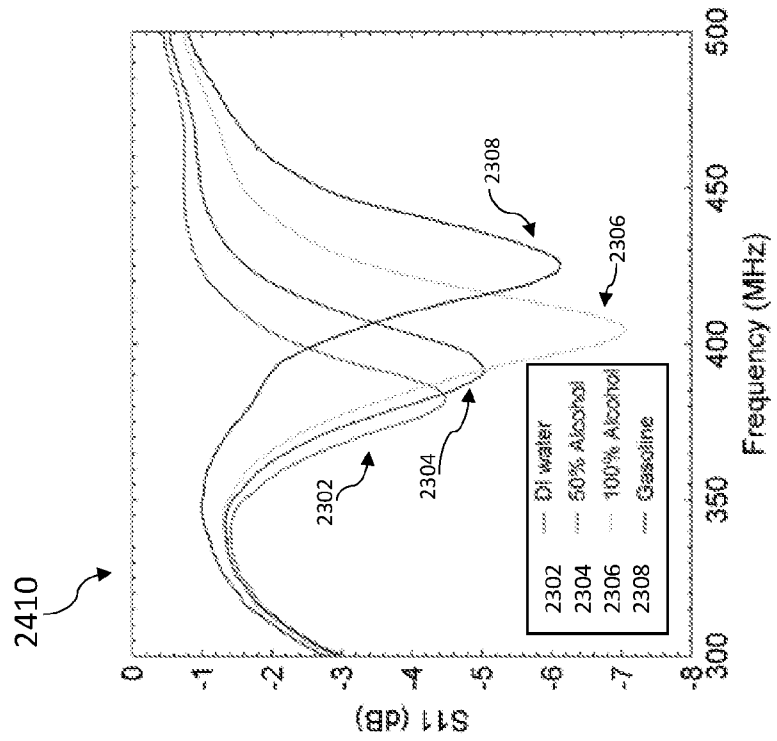
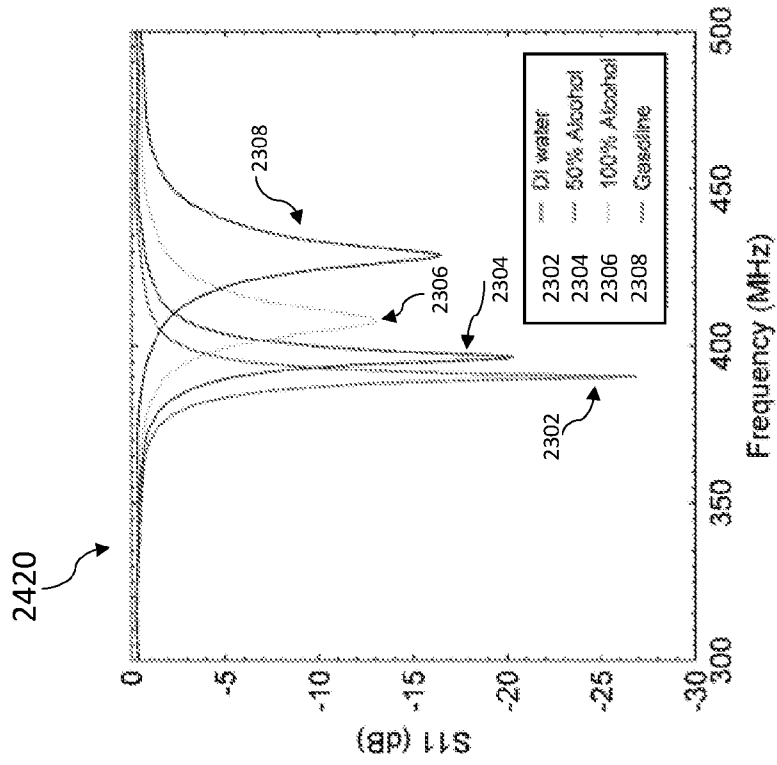


FIG. 24

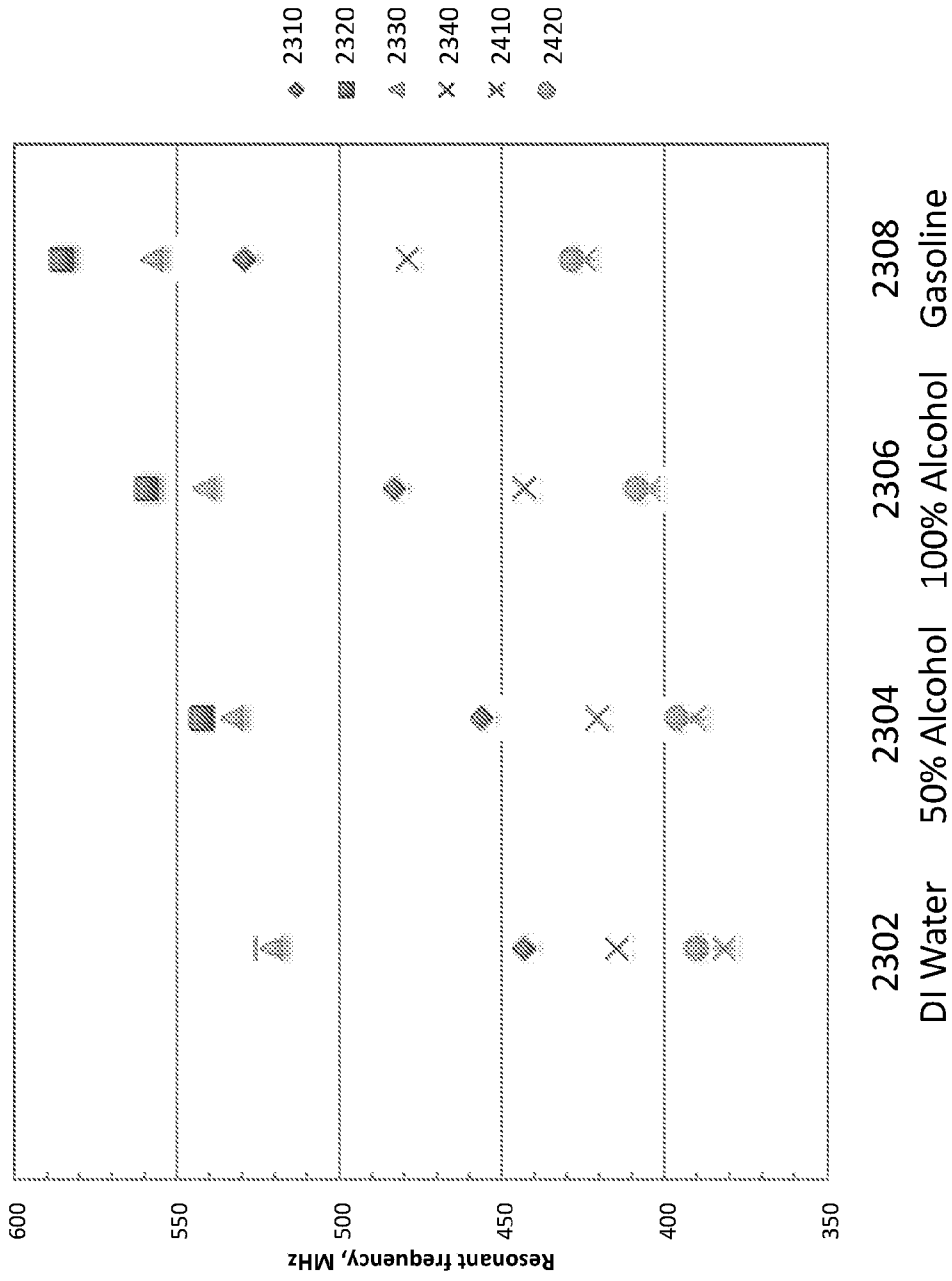


FIG. 25

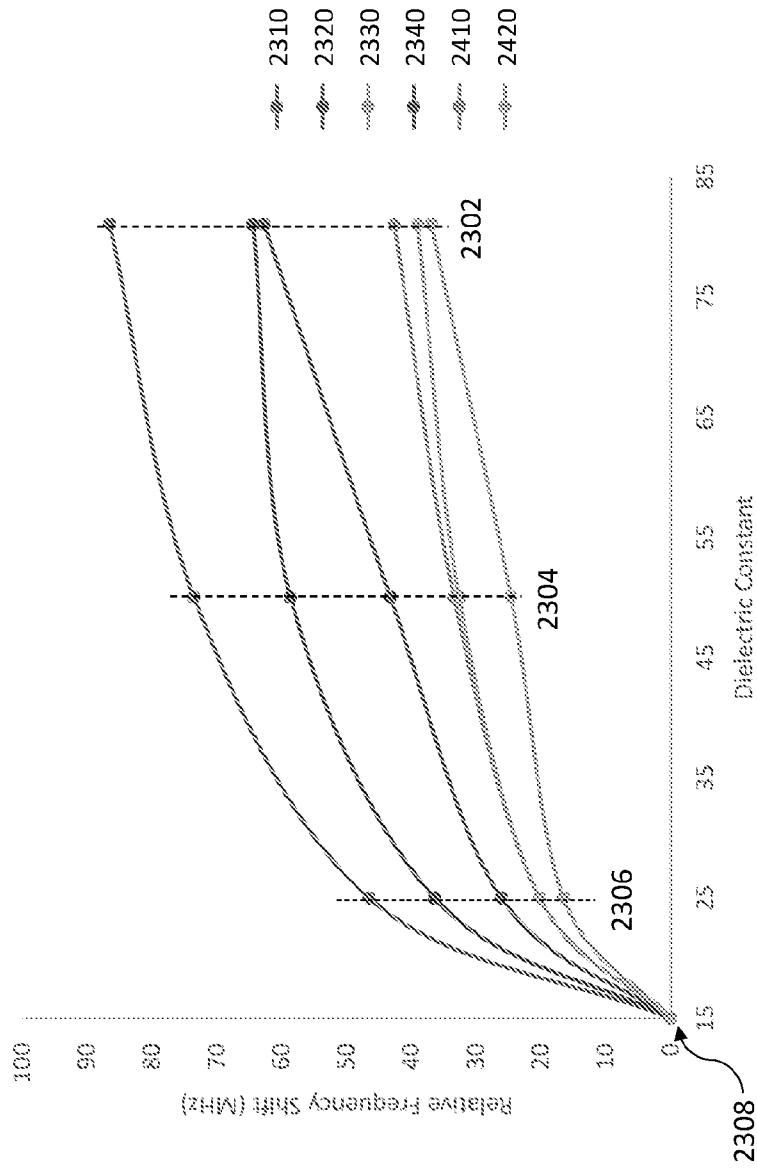


FIG. 26

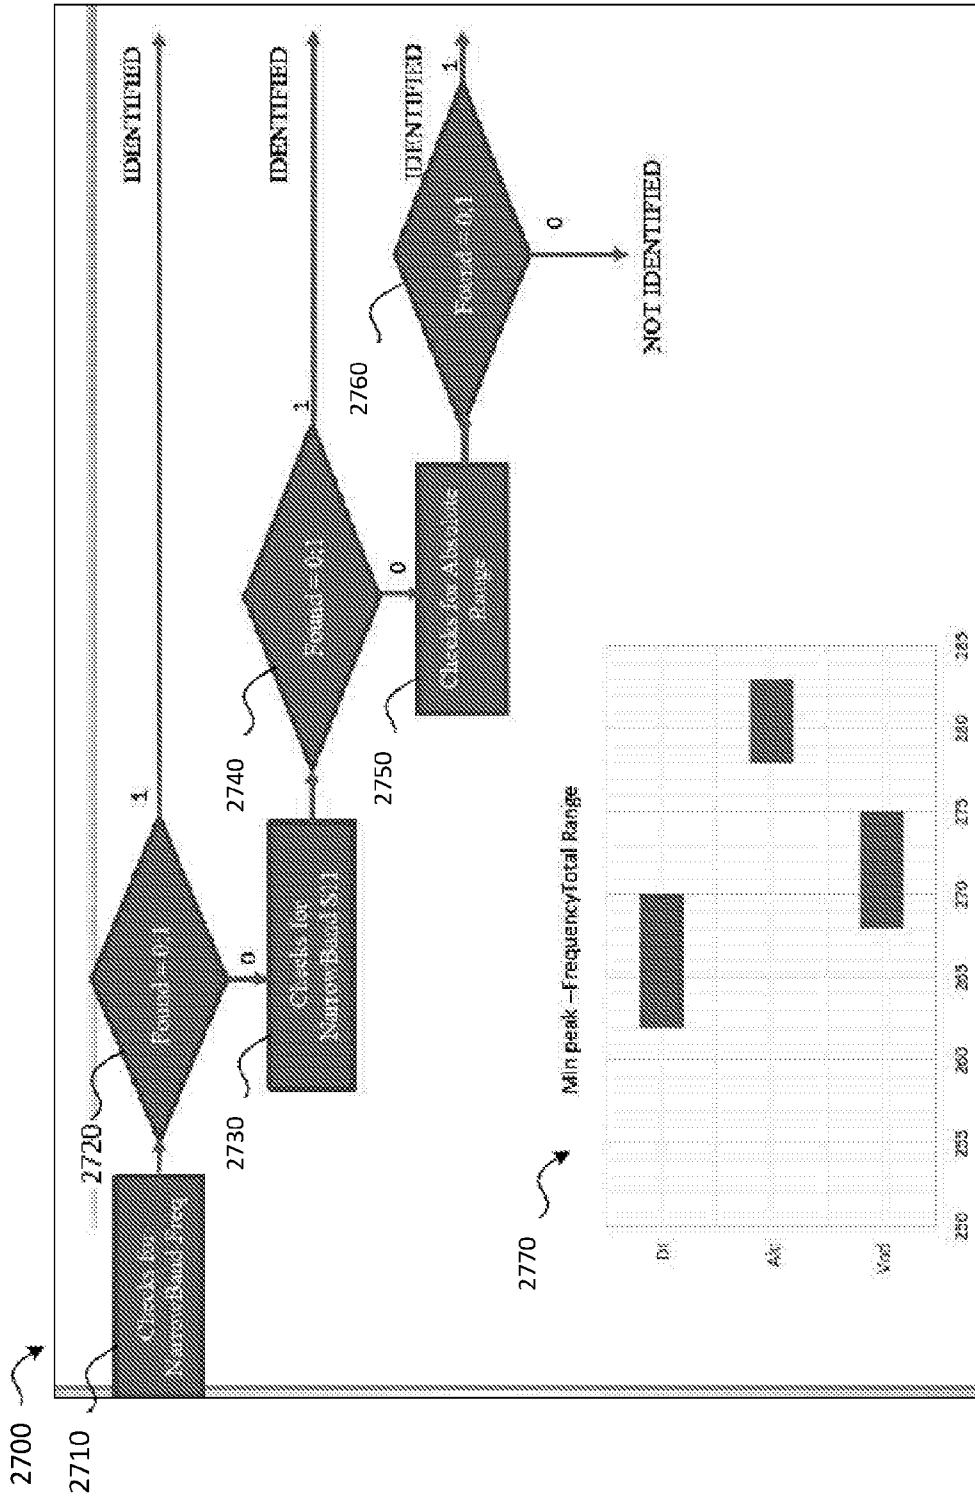


FIG. 27

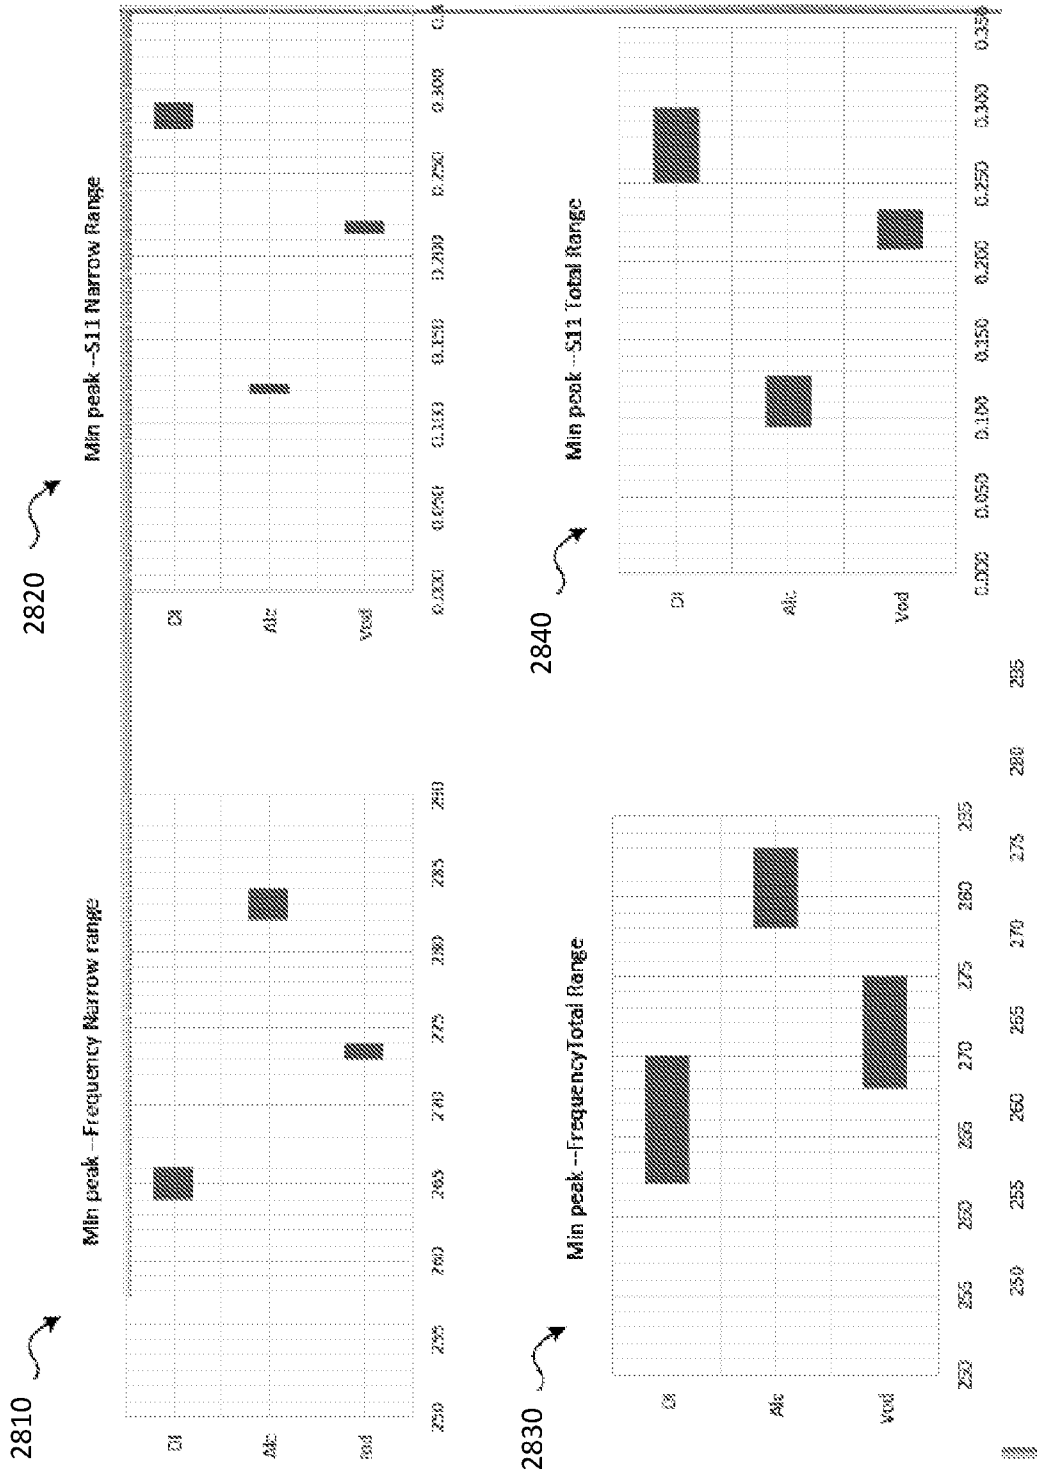


FIG. 28

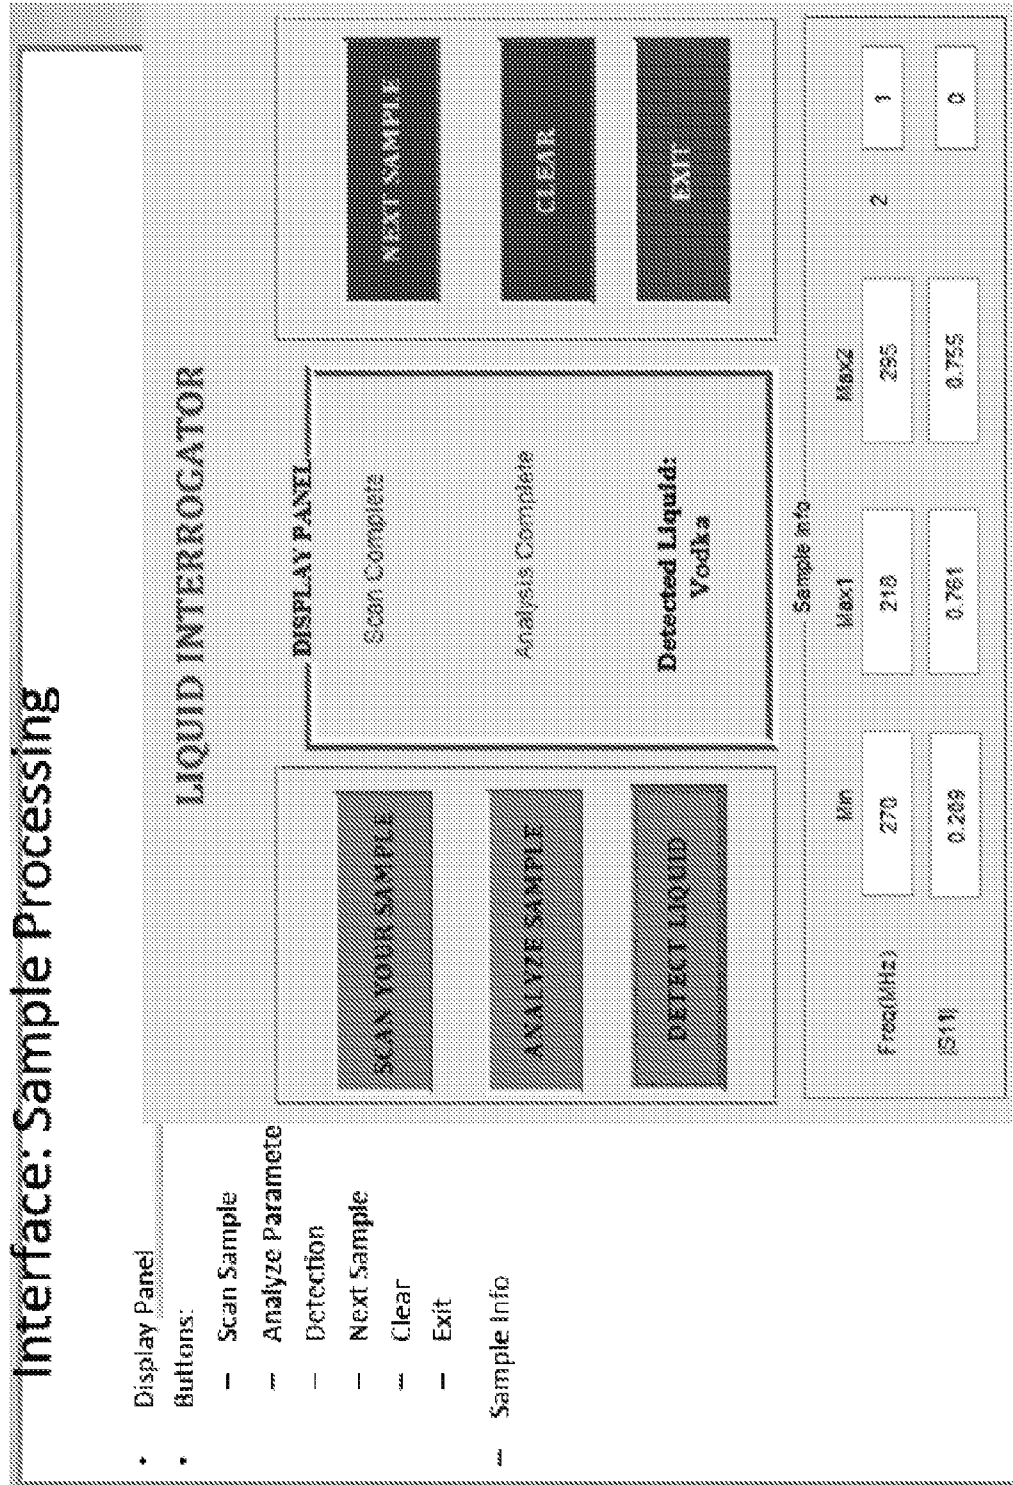


FIG. 29

Interface to control measurement parameters


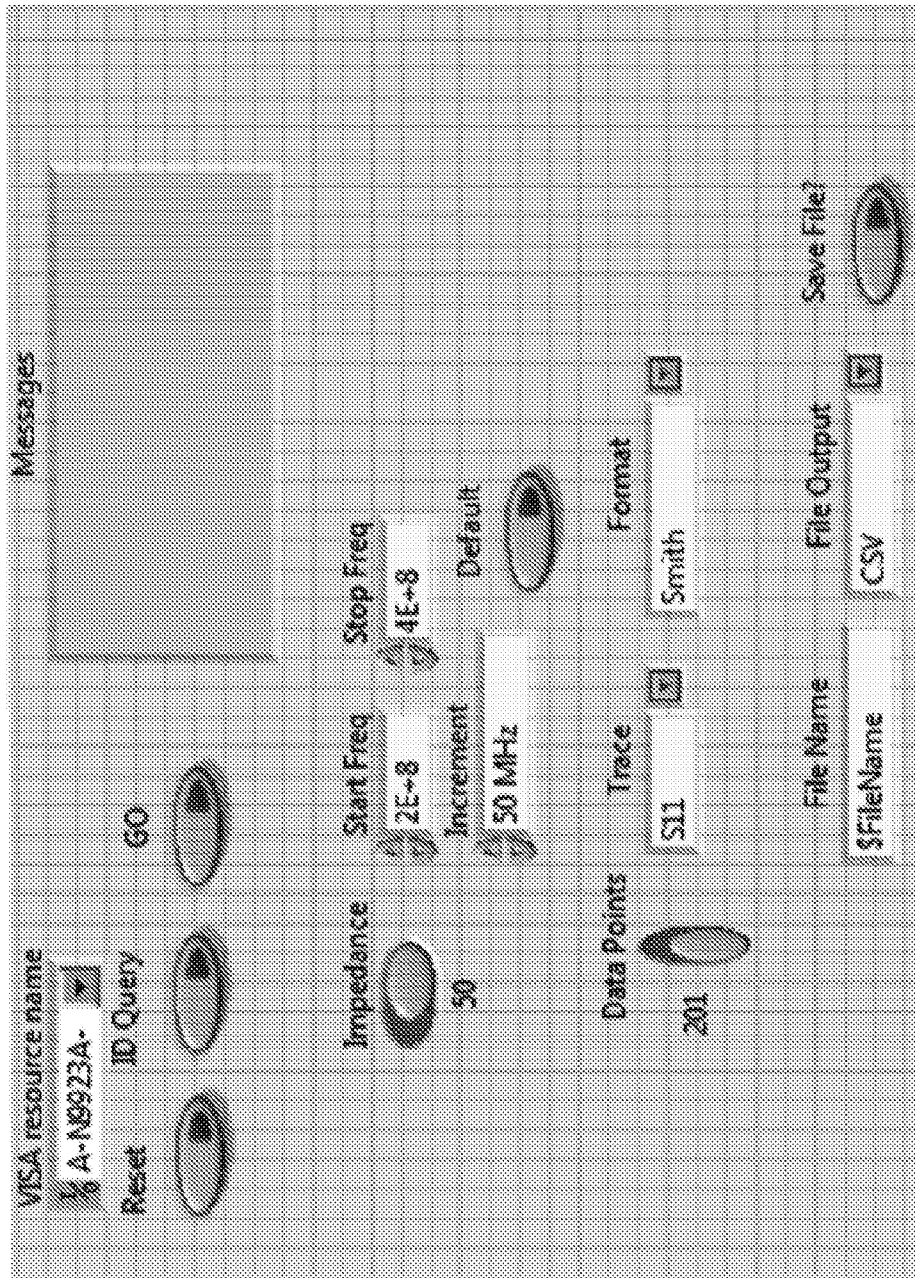


FIG. 30

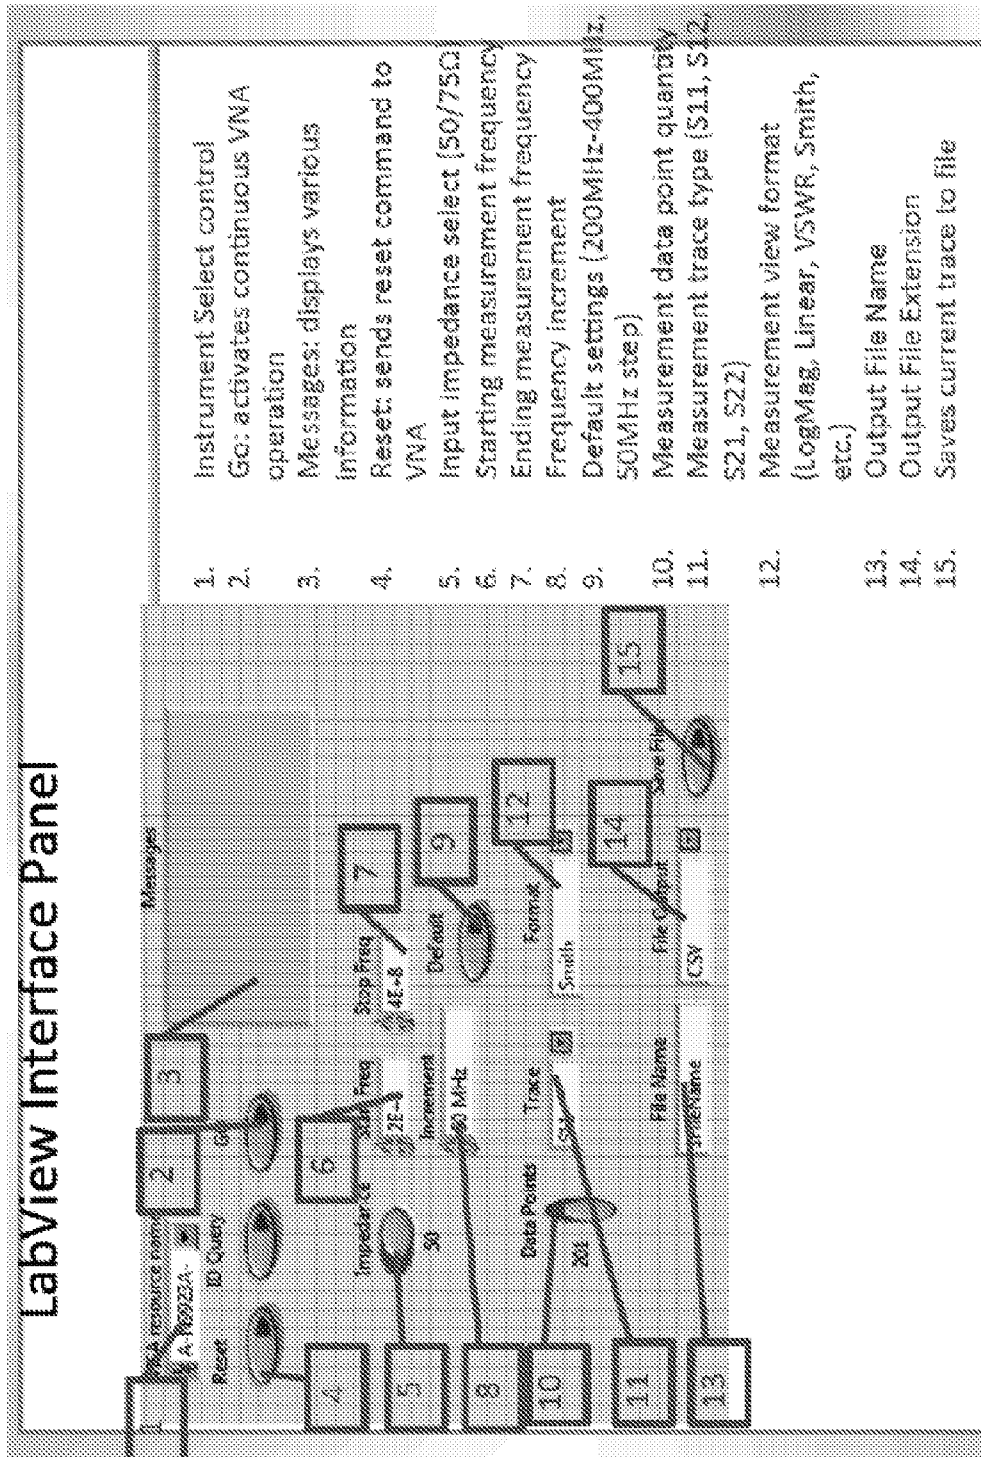

1. Instrument Select control
2. Go: activates continuous VNA operation
3. Messages: displays various information
4. Reset: sends reset command to VNA
5. Input impedance select (50/75Ω)
6. Starting measurement frequency
7. Ending measurement frequency
8. Frequency increment
9. Default settings (200MHz-400MHz, 50MHz step)
10. Measurement data point quantity
11. Measurement trace type (S11, S12, S21, S22)
12. Measurement view format (LogMag, Linear, VSWR, Smith, etc.)
13. Output File Name
14. Output File Extension
15. Saves current trace to file

FIG. 31

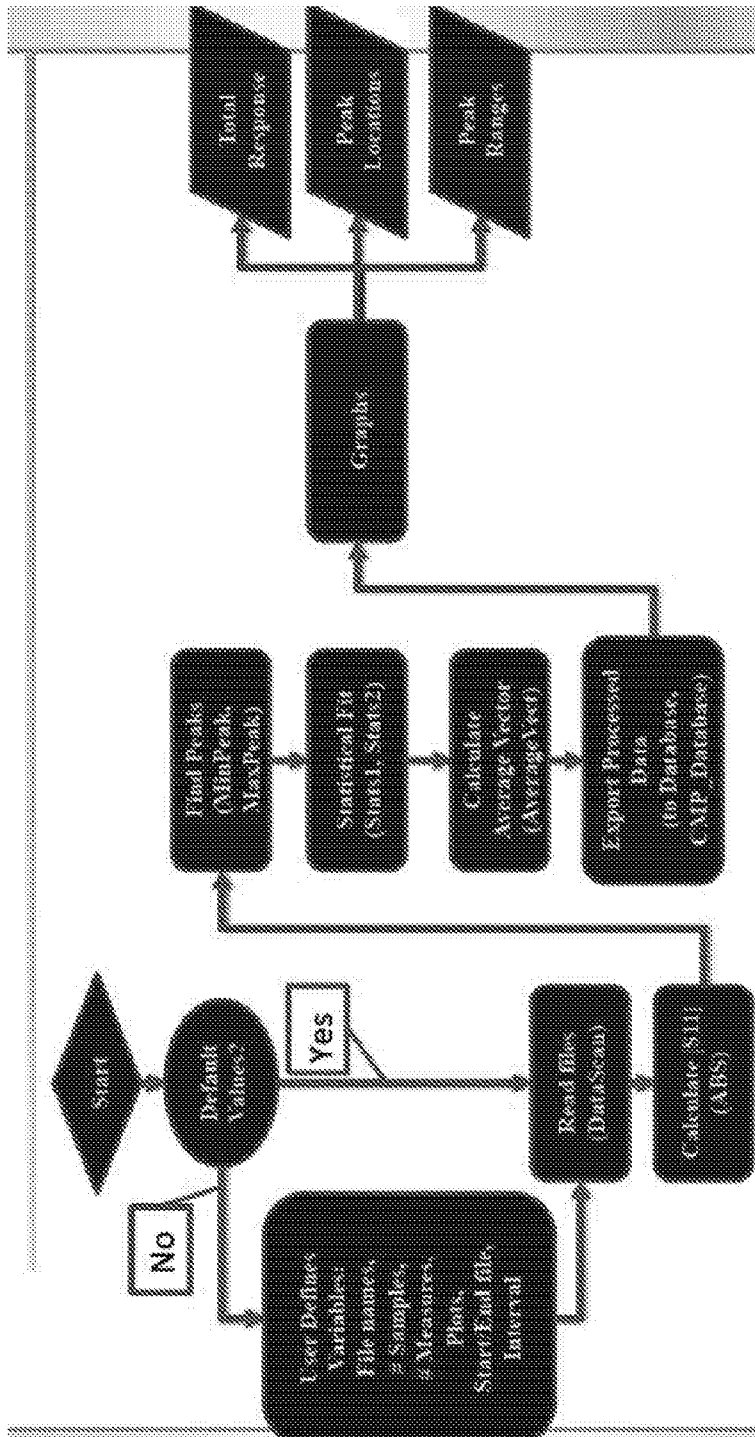


FIG. 34

INTERNATIONAL SEARCH REPORT

International application No.

PCT/ISA/210/17/046024

Box No. II Observations where certain claims were found unsearchable (Continuation of item 2 of first sheet)

This international search report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons:

1. Claims Nos.:
because they relate to subject matter not required to be searched by this Authority, namely:

2. Claims Nos.:
because they relate to parts of the international application that do not comply with the prescribed requirements to such an extent that no meaningful international search can be carried out, specifically:

3. Claims Nos.: 7-20, 26-41, 47-49
because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a).

Box No. III Observations where unity of invention is lacking (Continuation of item 3 of first sheet)

This International Searching Authority found multiple inventions in this international application, as follows:

1. As all required additional search fees were timely paid by the applicant, this international search report covers all searchable claims.
2. As all searchable claims could be searched without effort justifying additional fees, this Authority did not invite payment of additional fees.
3. As only some of the required additional search fees were timely paid by the applicant, this international search report covers only those claims for which fees were paid, specifically claims Nos.:

4. No required additional search fees were timely paid by the applicant. Consequently, this international search report is restricted to the invention first mentioned in the claims; it is covered by claims Nos.:

Remark on Protest

- The additional search fees were accompanied by the applicant's protest and, where applicable, the payment of a protest fee.
- The additional search fees were accompanied by the applicant's protest but the applicable protest fee was not paid within the time limit specified in the invitation.
- No protest accompanied the payment of additional search fees.

INTERNATIONAL SEARCH REPORT

International application No.

PCT/US2017/046024

A. CLASSIFICATION OF SUBJECT MATTER
 IPC(8) - A61B 5/00; A61B 5/08; A61B 5/113 (2017.01)
 CPC - A61B 5/06; A61B-005/06/2; A61B-005/107/3; A61B-005/113/5; G01N-033/00/31; H04Q 9/00 (2017.08)

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

See Search History document

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

USPC - 29/601.000; 73/23.200; 73/24.010; 73/53.050; 600/534.000 (keyword delimited)

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

See Search History document

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y	US 20100164513 A1 (RAPOPORT) 01 July 2010 (01.07.2010) entire document	1-6, 21-25, 42-46
Y	US 5,549,008 A (BEAUDUCCEL et al) 27 August 1996 (27.08.1996) entire document	1-6, 21-25, 42-46
Y	US 20060025664 A1 (KIM et al) 02 February 2006 (02.02.2006) entire document	25, 46
A	US 20050254058 A1 (ALPHONSE) 17 November 2005 (17.11.2005) entire document	1-6, 21-25, 42-46
A	US 20080203281 A1 (SANDERS et al) 28 August 2008 (28.08.2008) entire document	1-6, 21-25, 42-46
A	US 20070180892 A1 (SUNSHINE) 09 August 2007 (09.08.2007) entire document	1-6, 21-25, 42-46
A	US 2014/0187906 A1 (VoluSense AS) 03 July 2014 (03.07.2014) entire document	1-6, 21-25, 42-46

Further documents are listed in the continuation of Box C.

See patent family annex.

* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier application or patent but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search

03 October 2017

Date of mailing of the international search report

18 OCT 2017

Name and mailing address of the ISA/US

Mail Stop PCT, Attn: ISA/US, Commissioner for Patents
 P.O. Box 1450, Alexandria, VA 22313-1450

Facsimile No. 571-273-8300

Authorized officer

Blaine R. Copenheaver

PCT Helpdesk: 571-272-4300
 PCT OSP: 571-272-7774